

FIG. 1

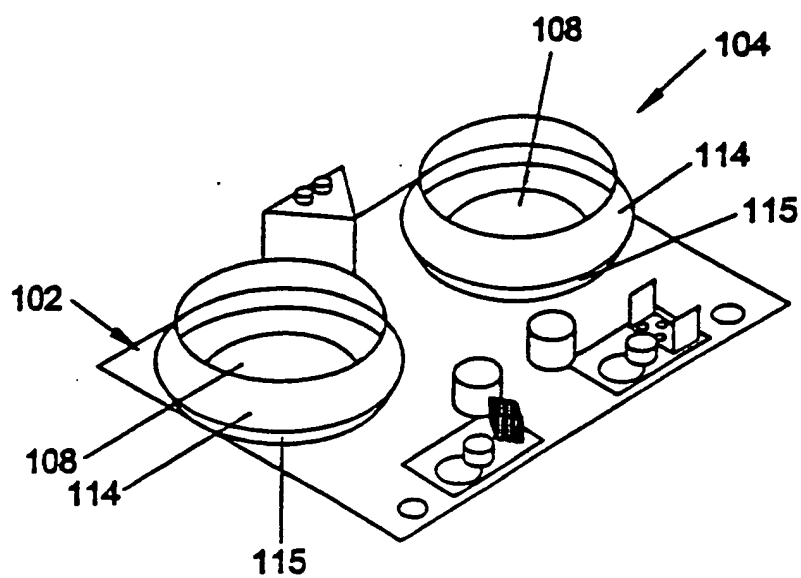


FIG. 2

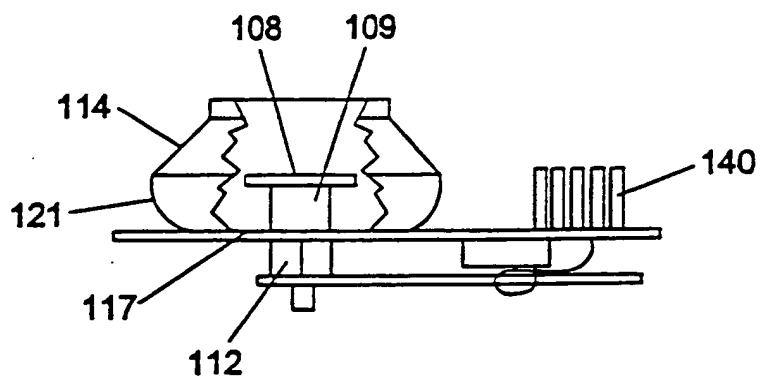


FIG. 3

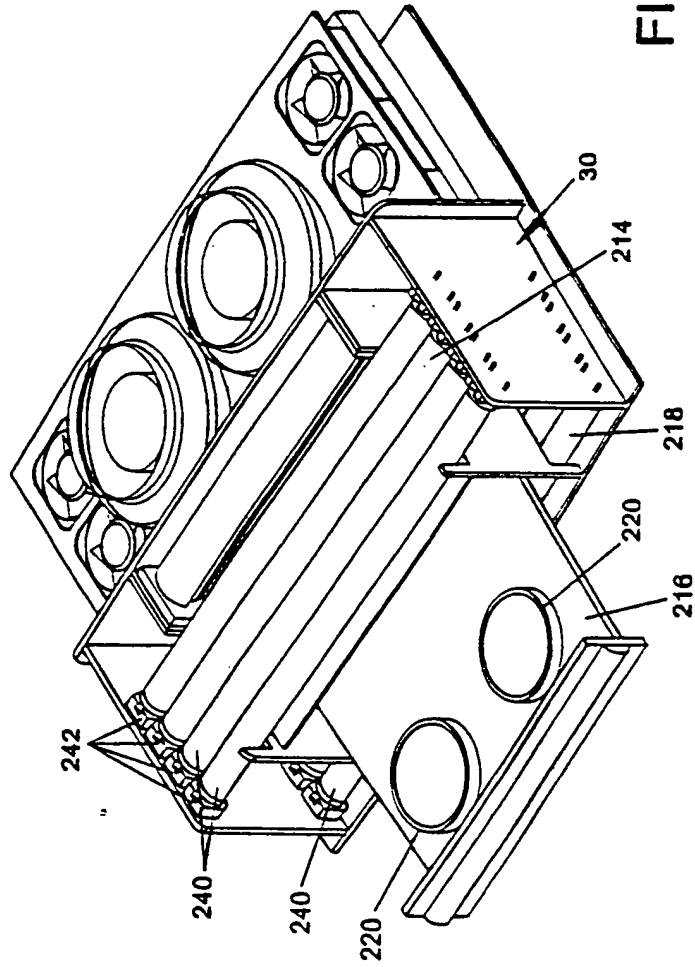


FIG. 4

102140-62783260

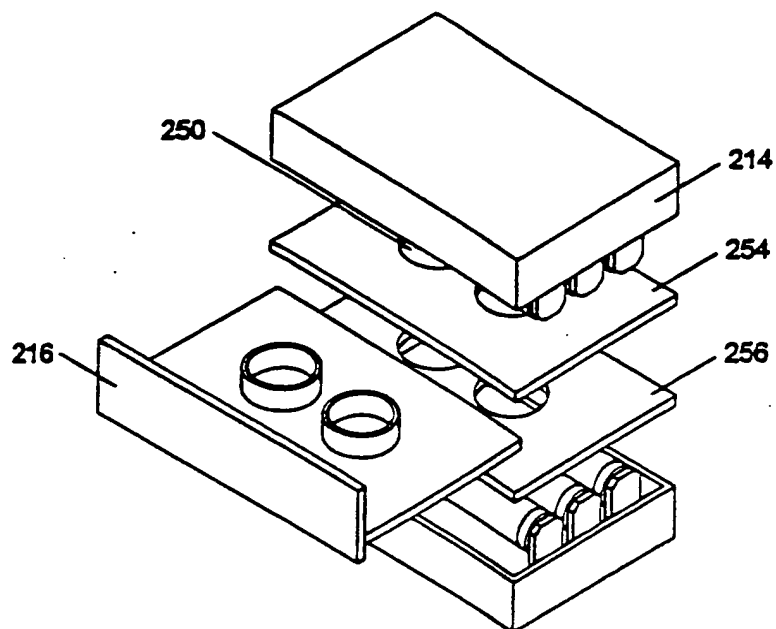


FIG. 5

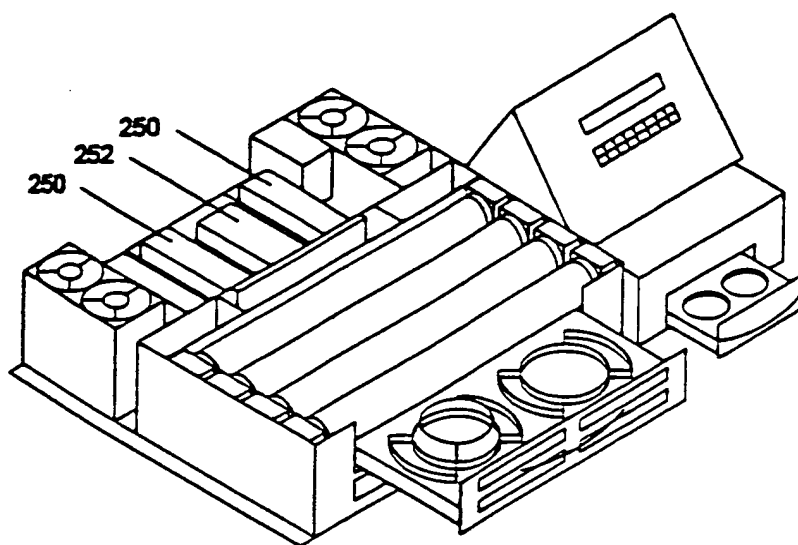


FIG. 6

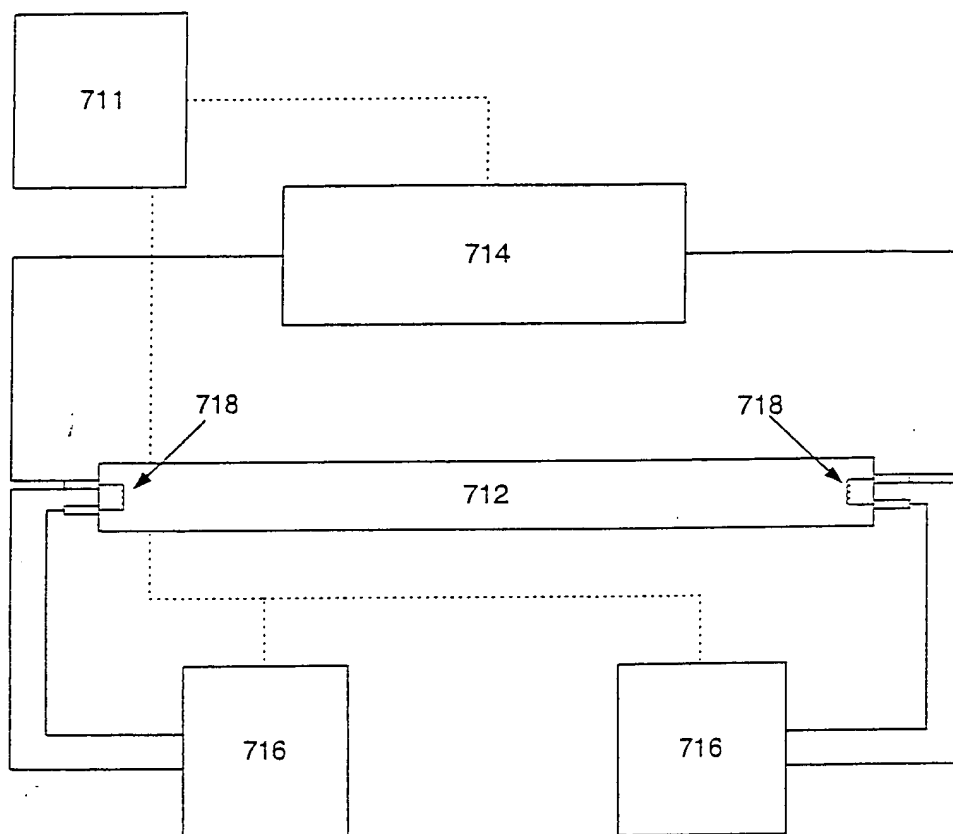


FIG. 7

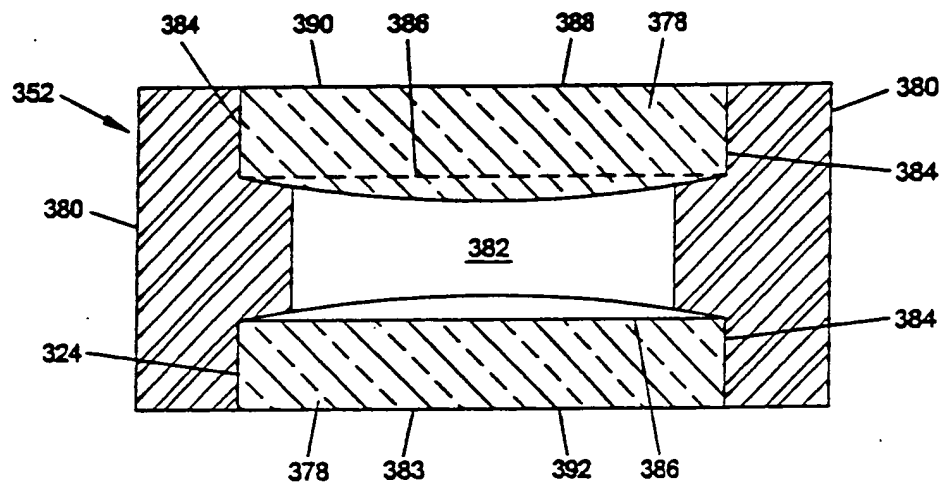


FIG. 8

FIG. 10

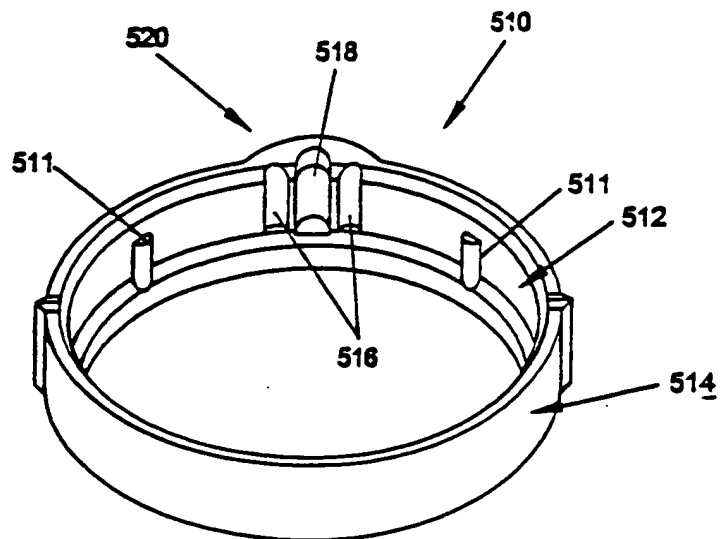


FIG. 9

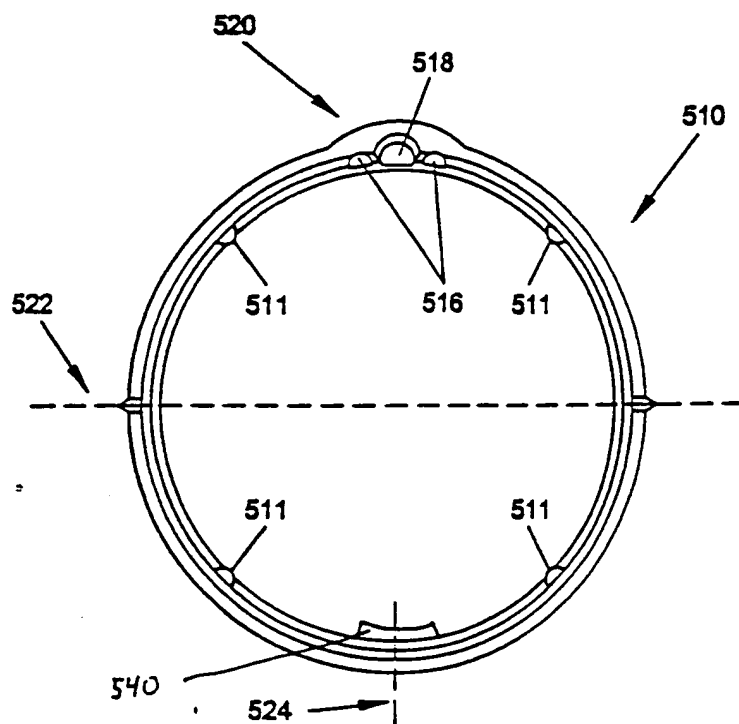


FIG. 10



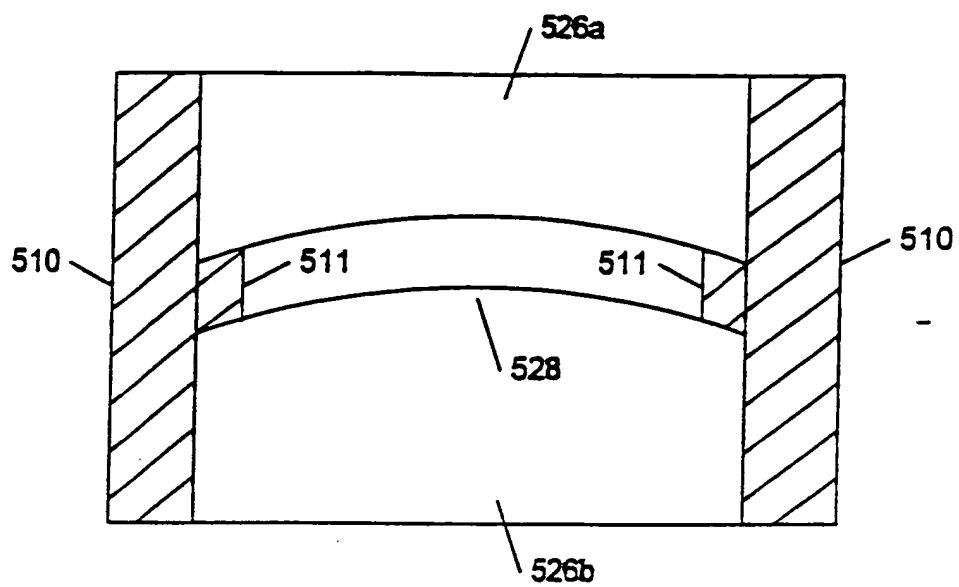


FIG. 11

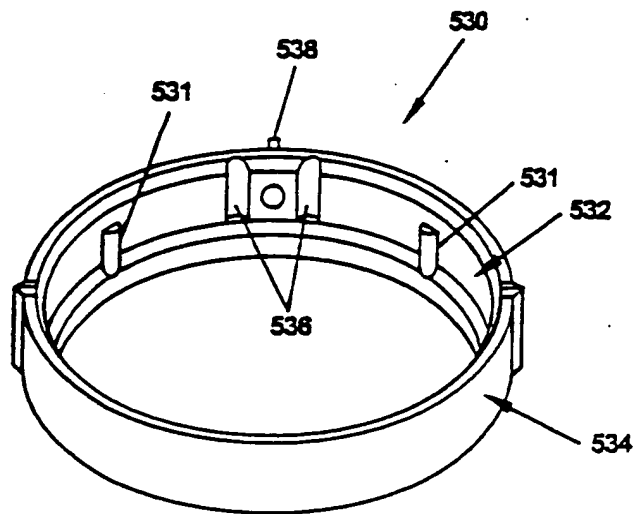


FIG. 12

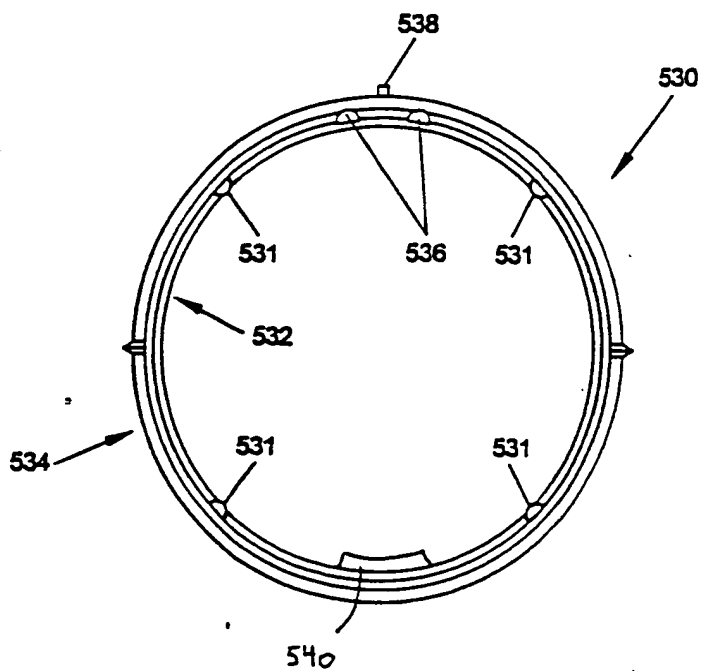


FIG. 13

09788439-071201  
FIG. 14

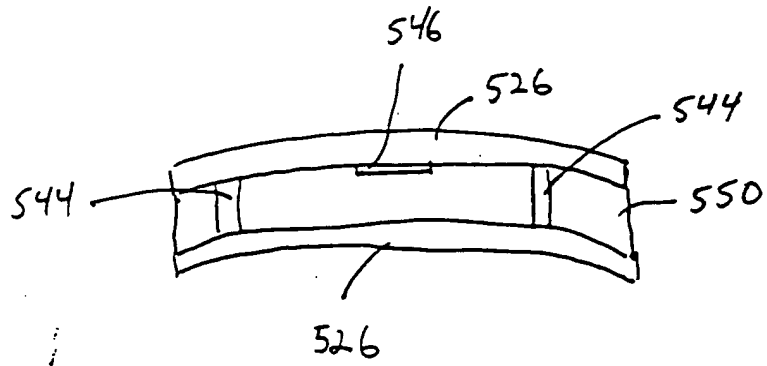


FIG. 14

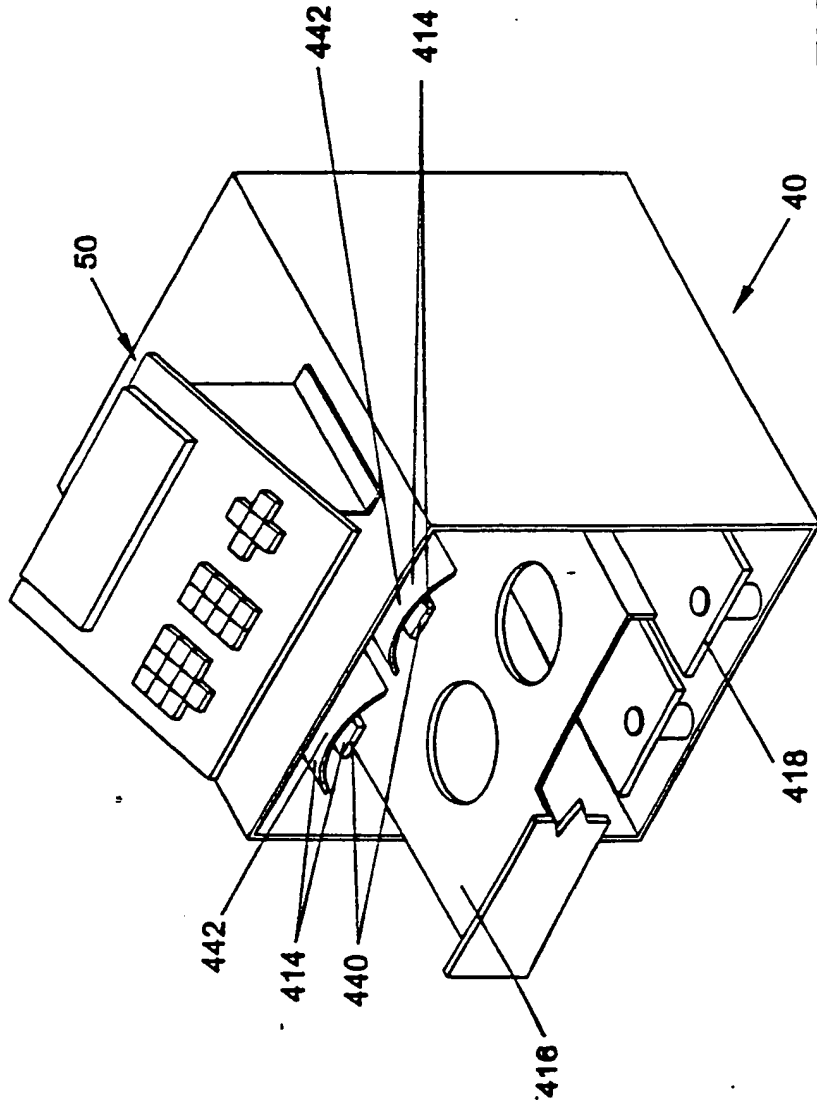


FIG. 15

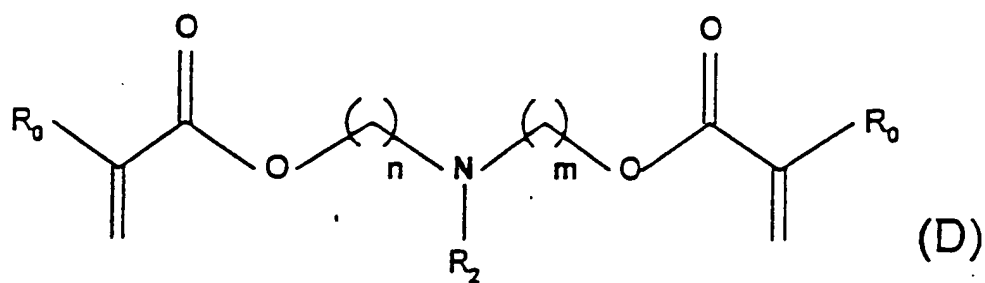
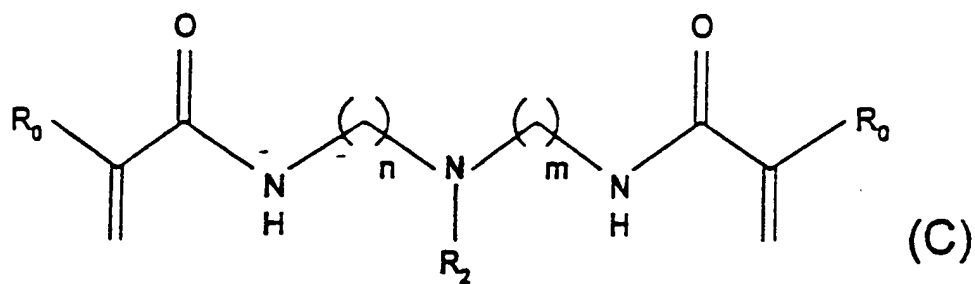
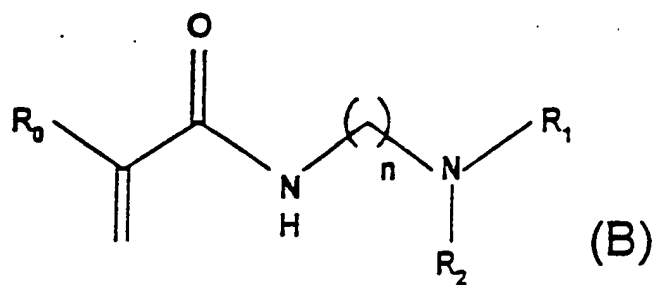
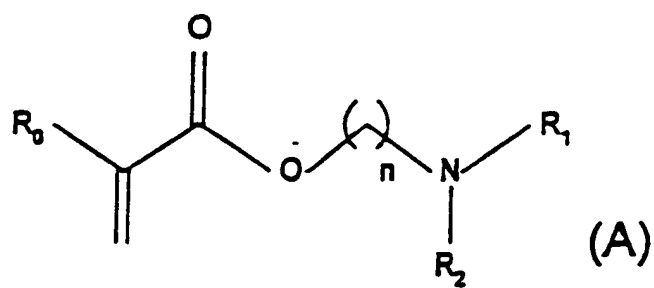


FIG. 16

FIG. 17

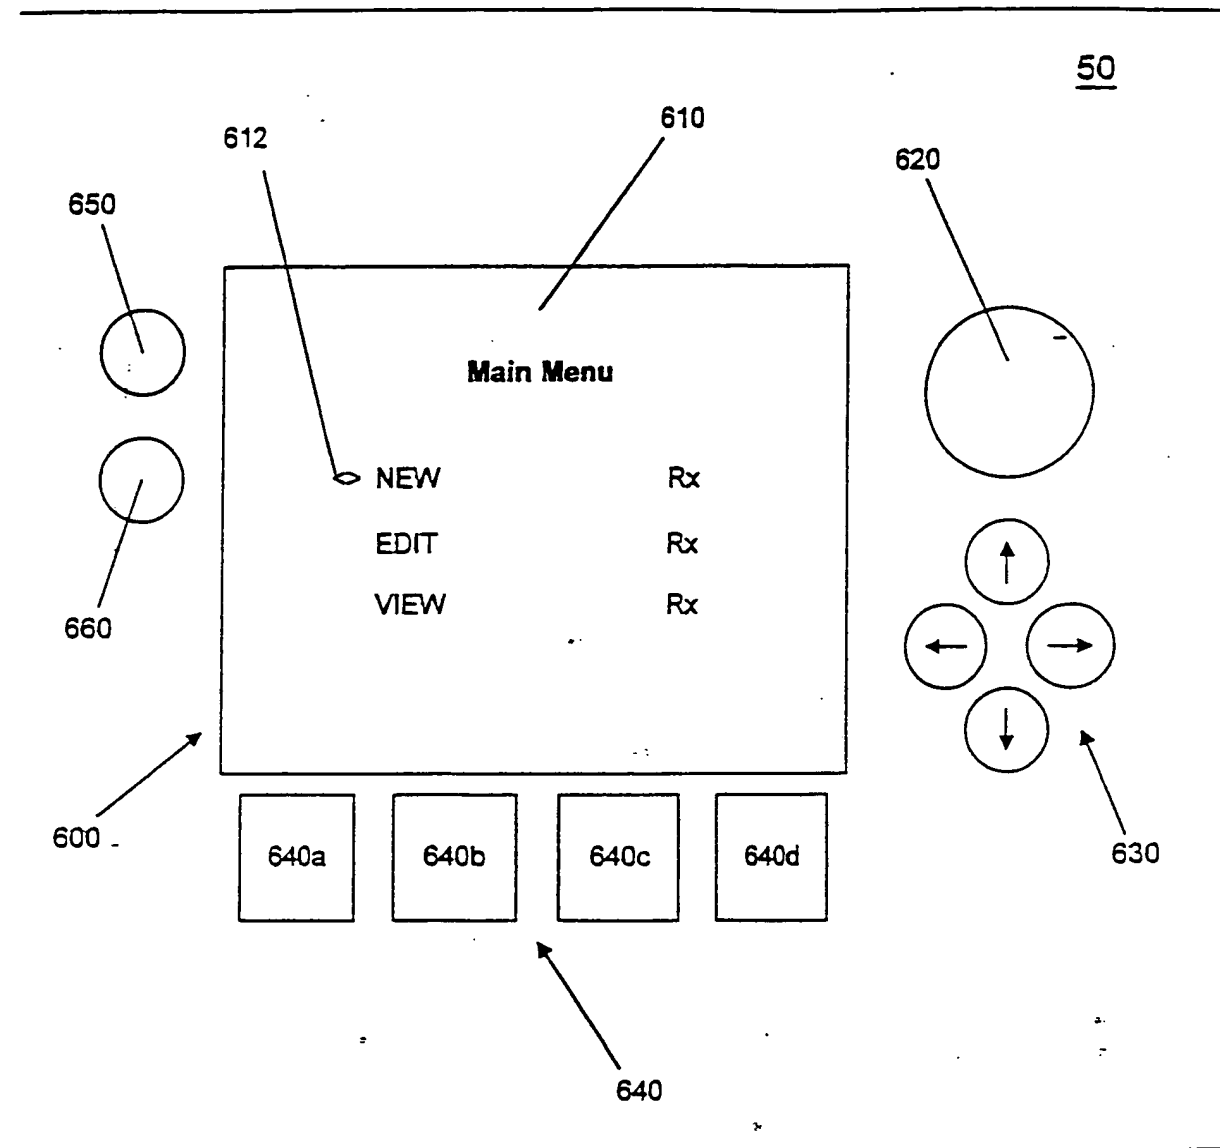


FIG. 17

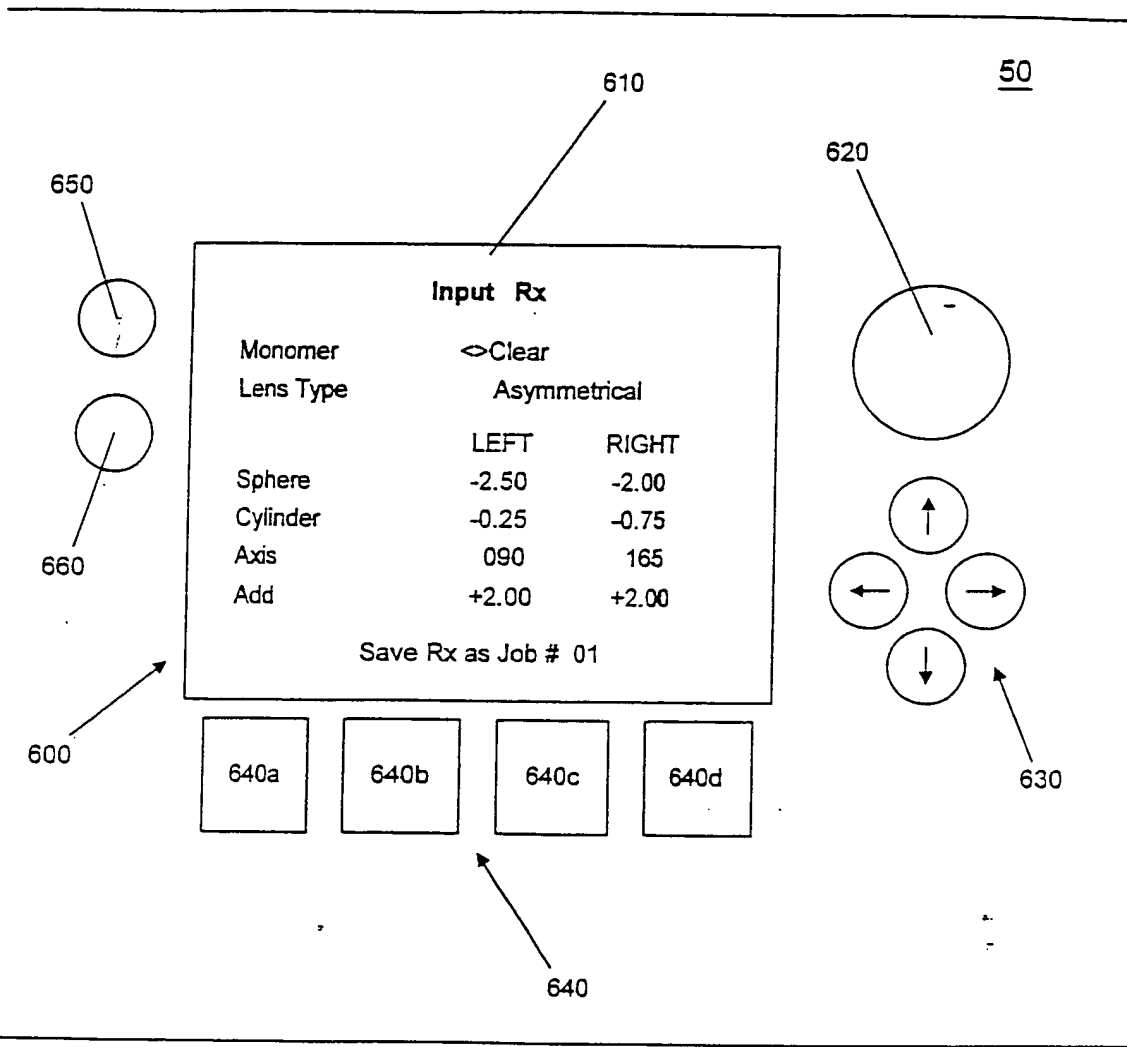


FIG. 18

FIG. 19

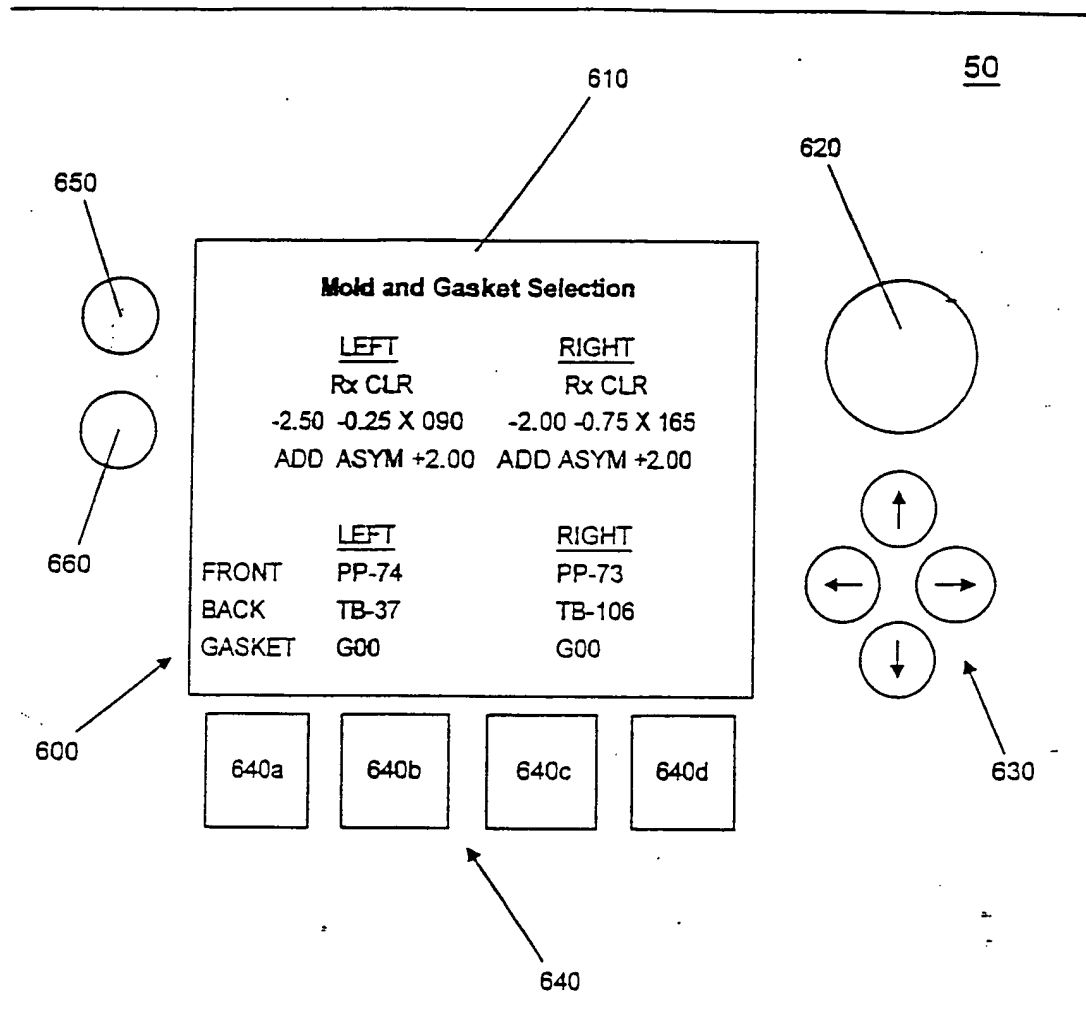
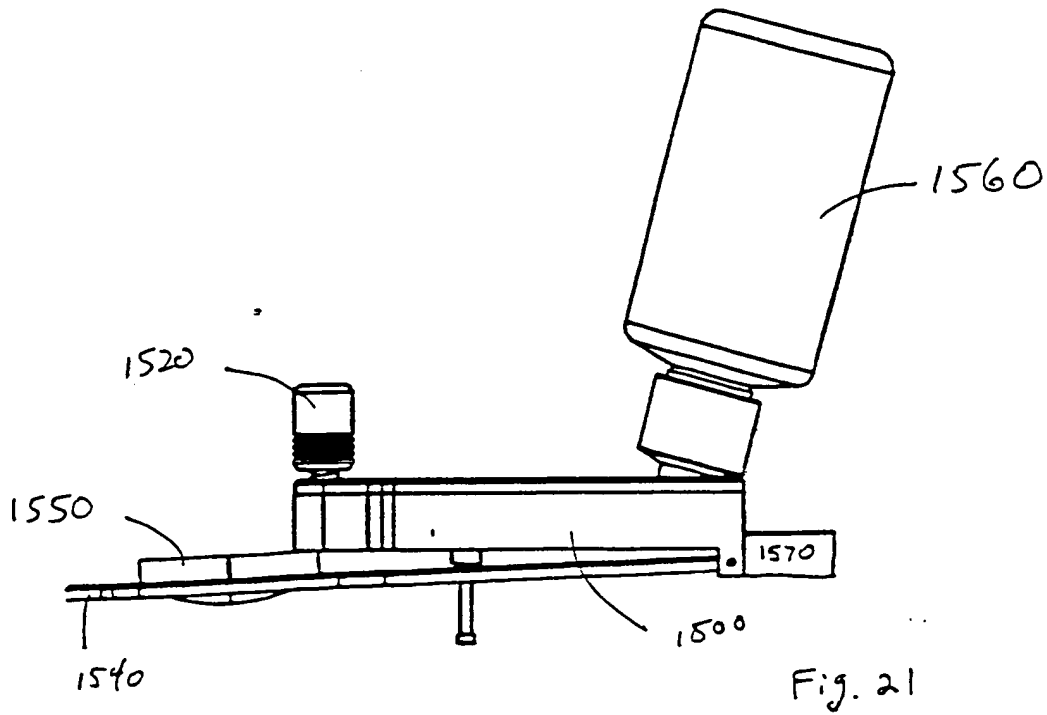
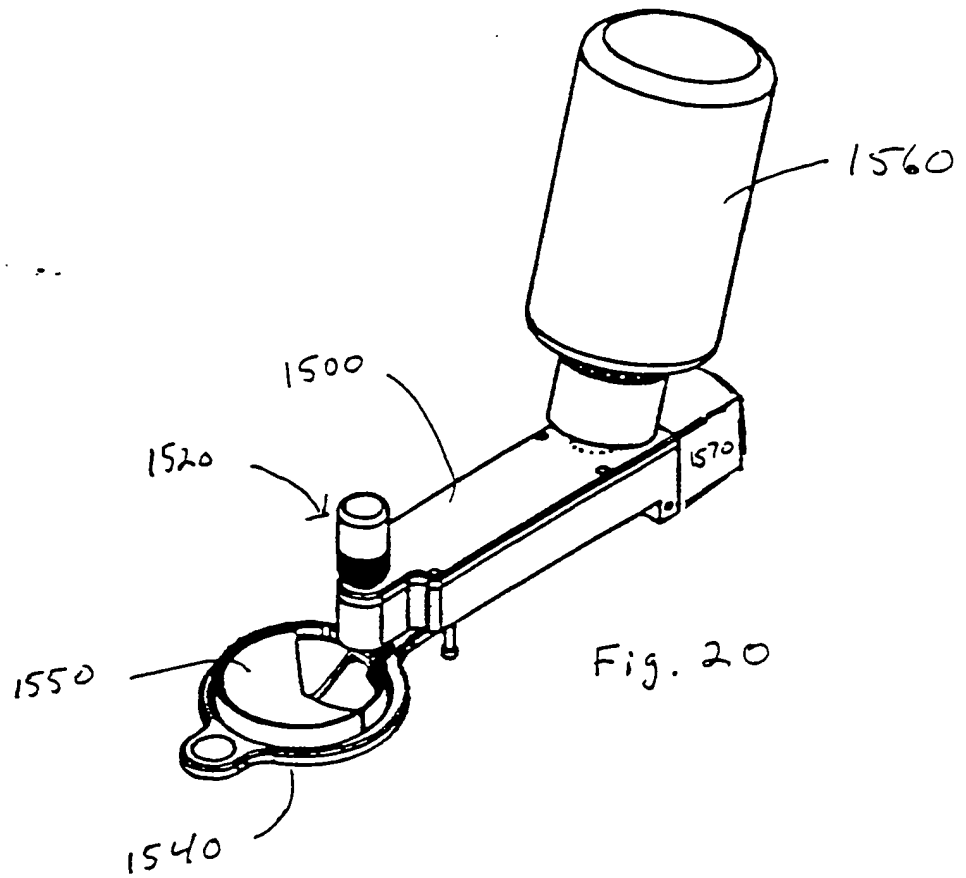


FIG. 19



FIG. 20





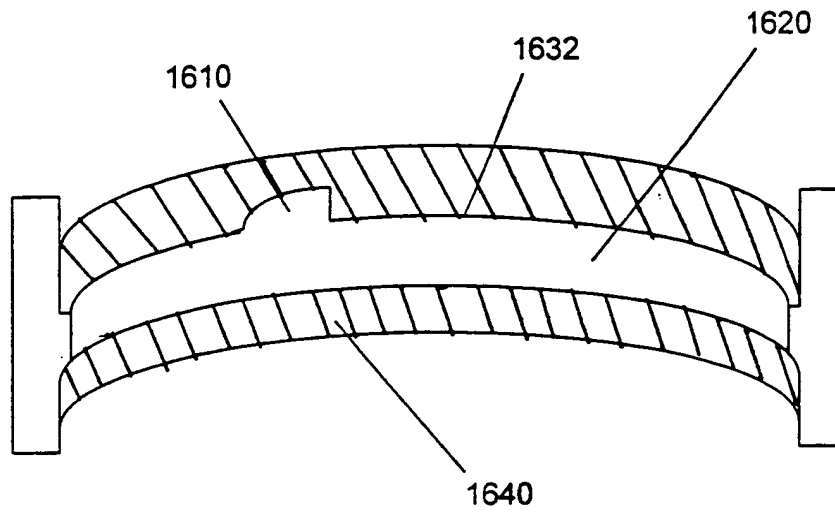


FIG. 24

FIG. 25

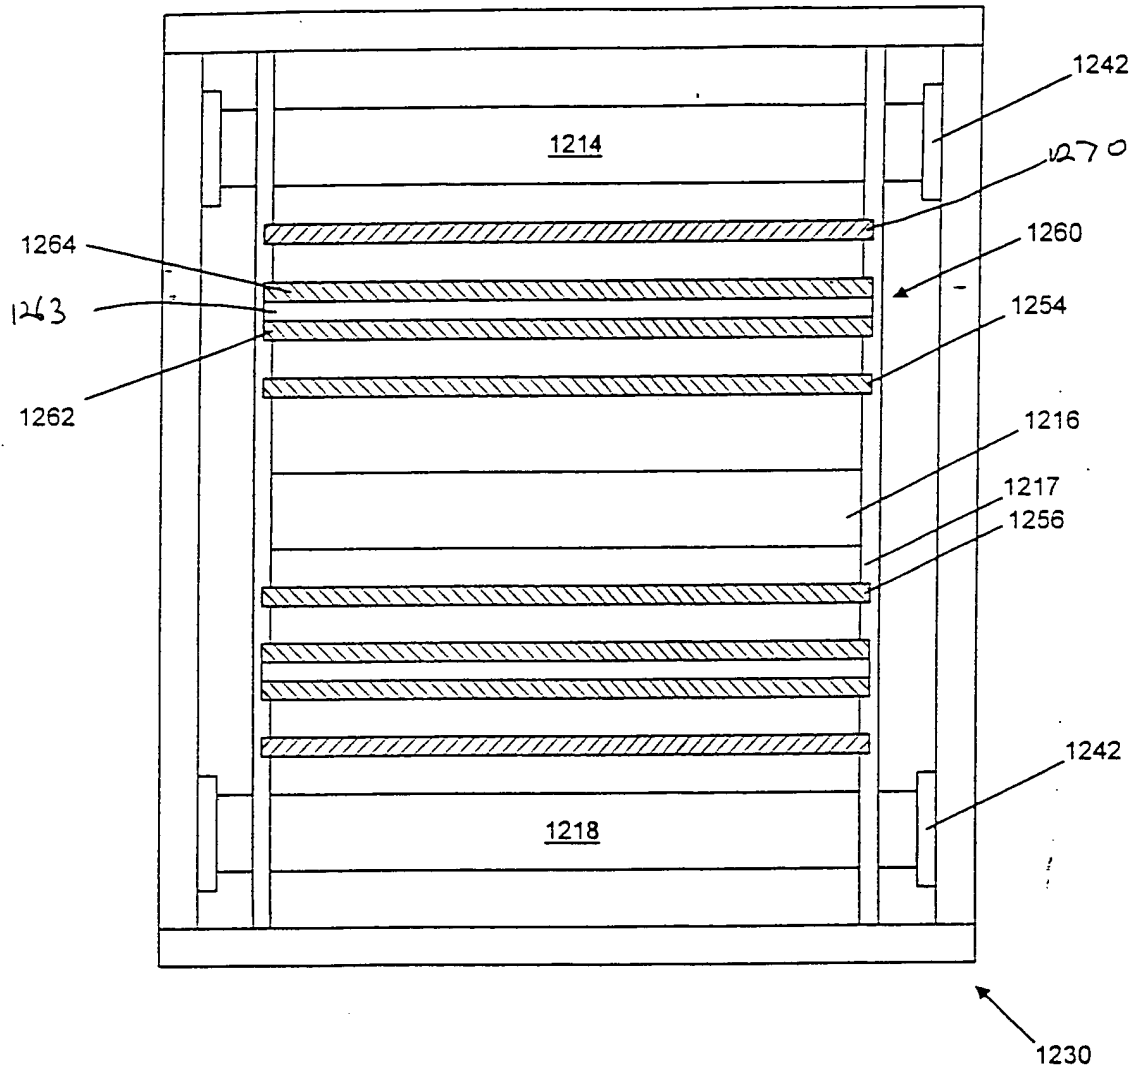


FIG. 25

FIG. 26

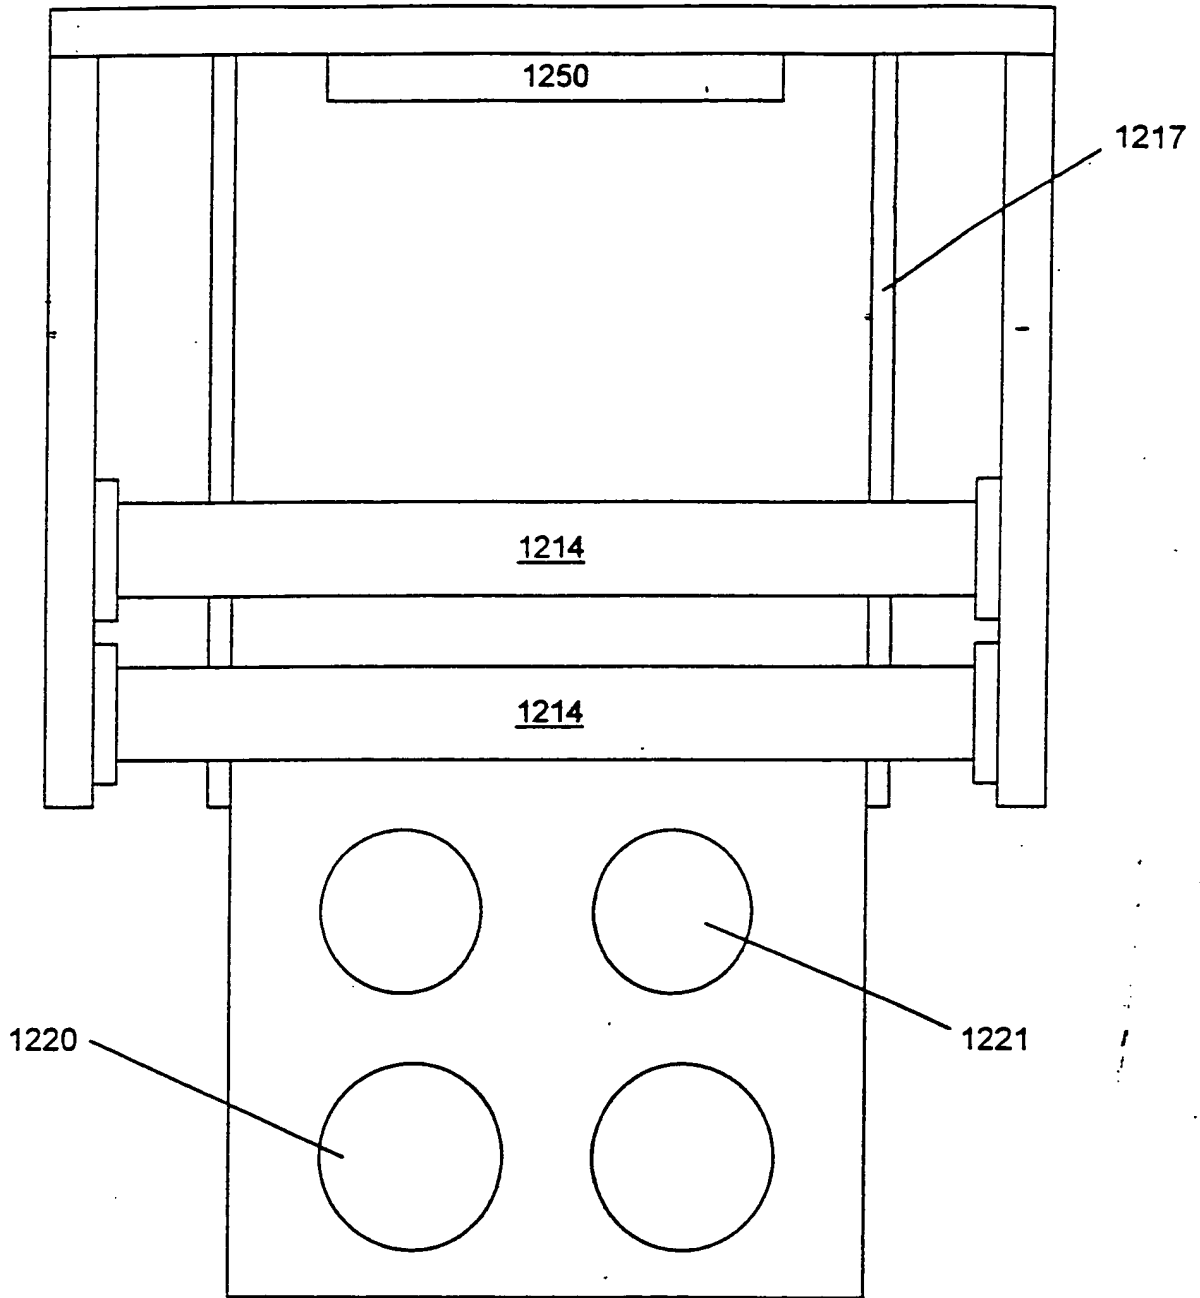


FIG. 26

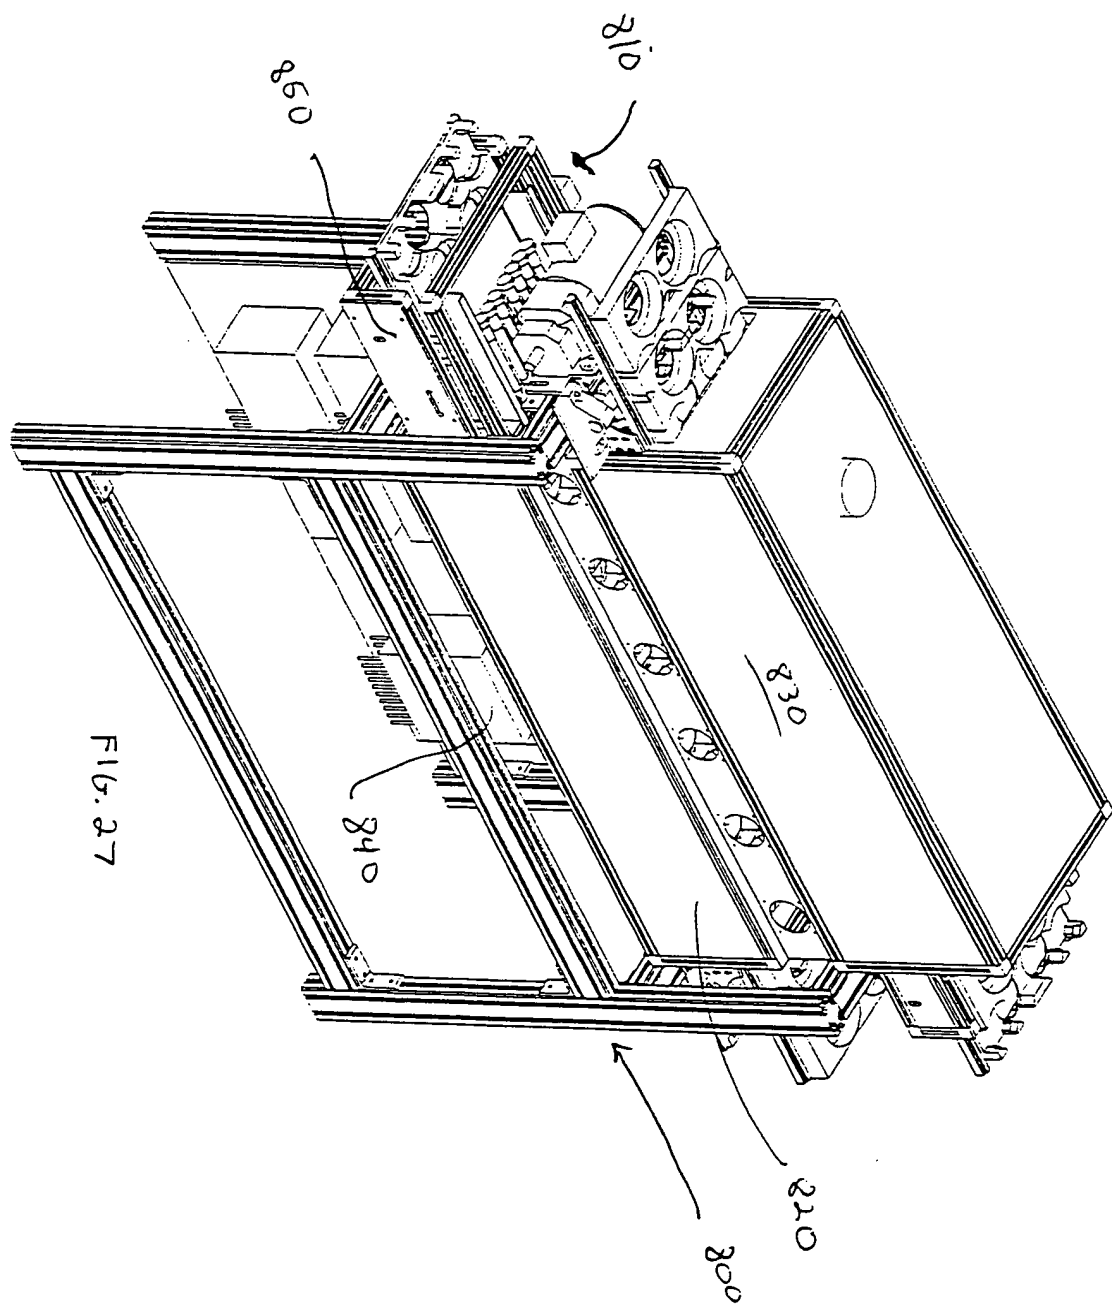


FIG. 27

09788439:071201

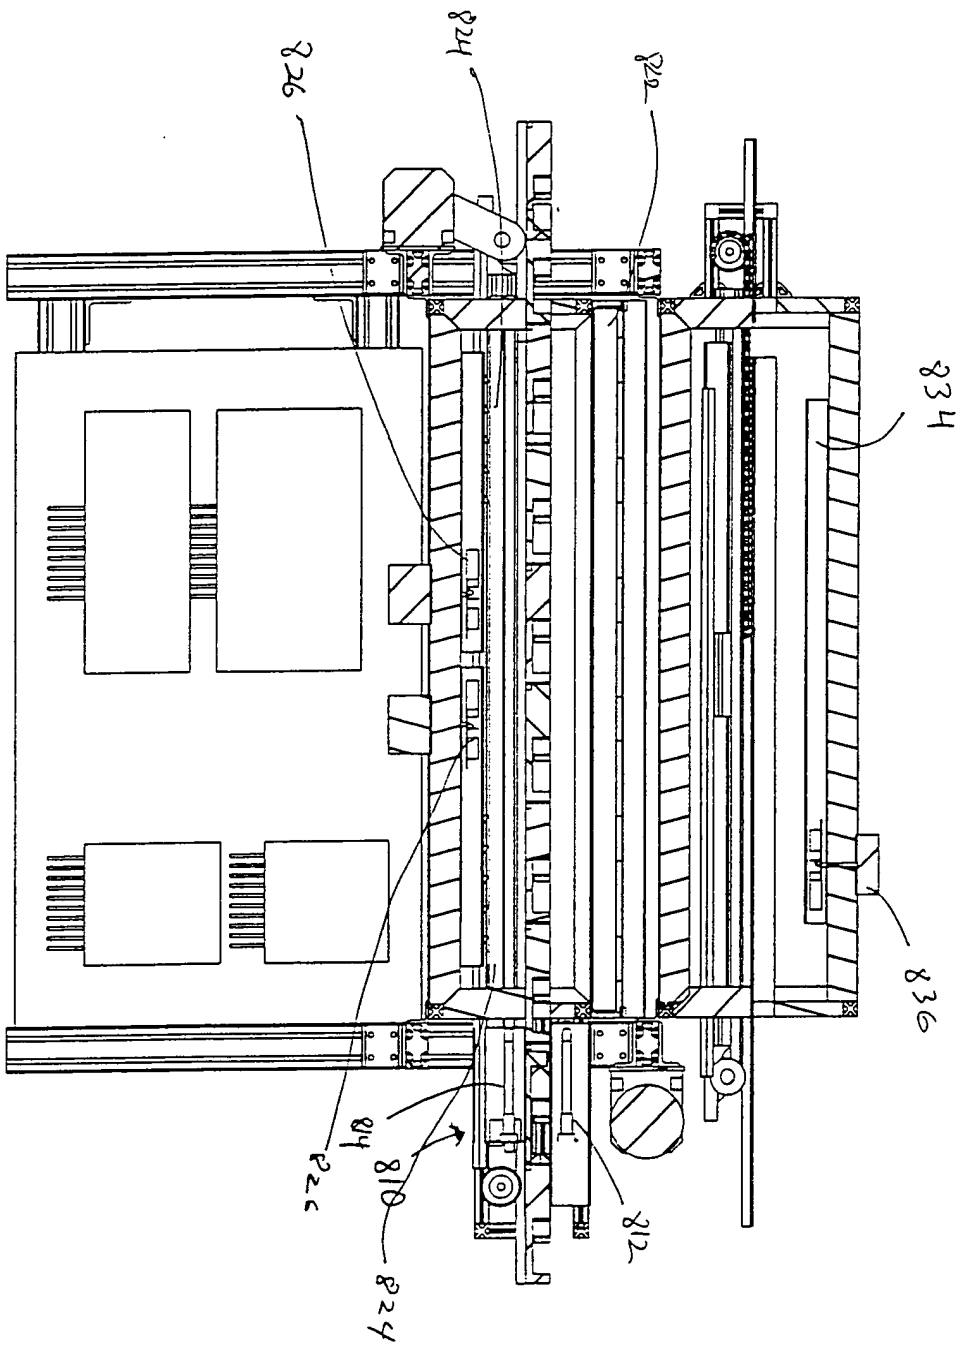


FIG 28

09788439-071201

FIG. 29

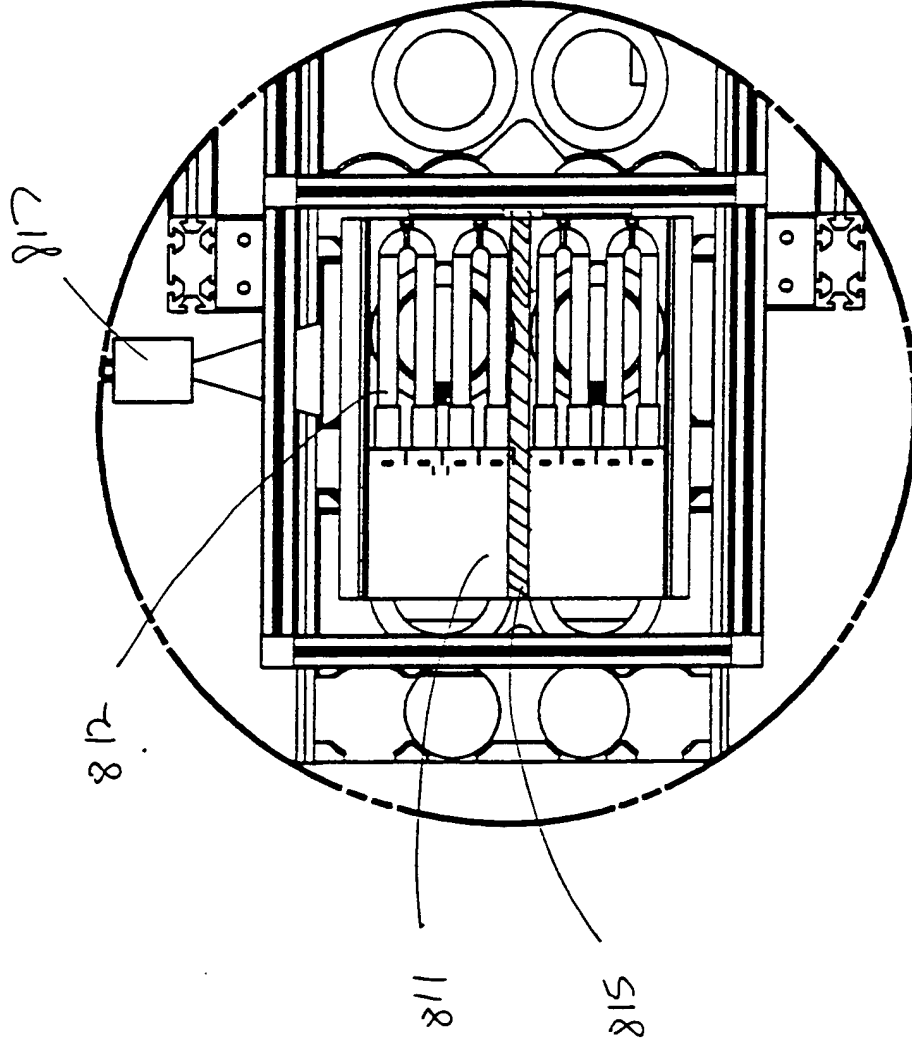


FIG. 29



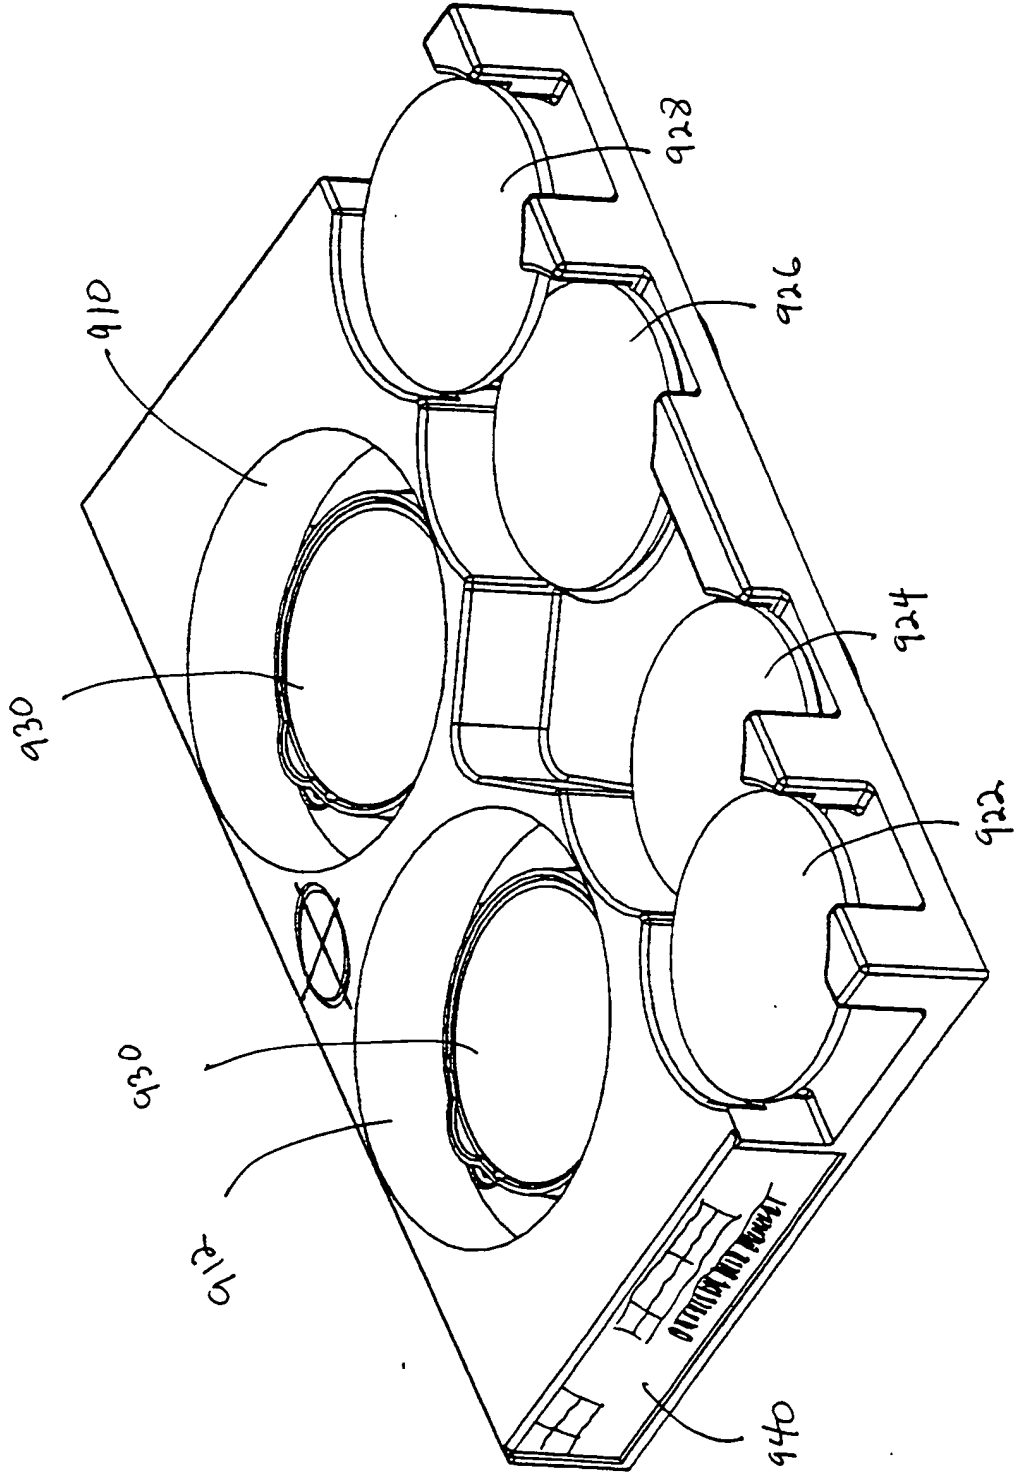


FIG. 30

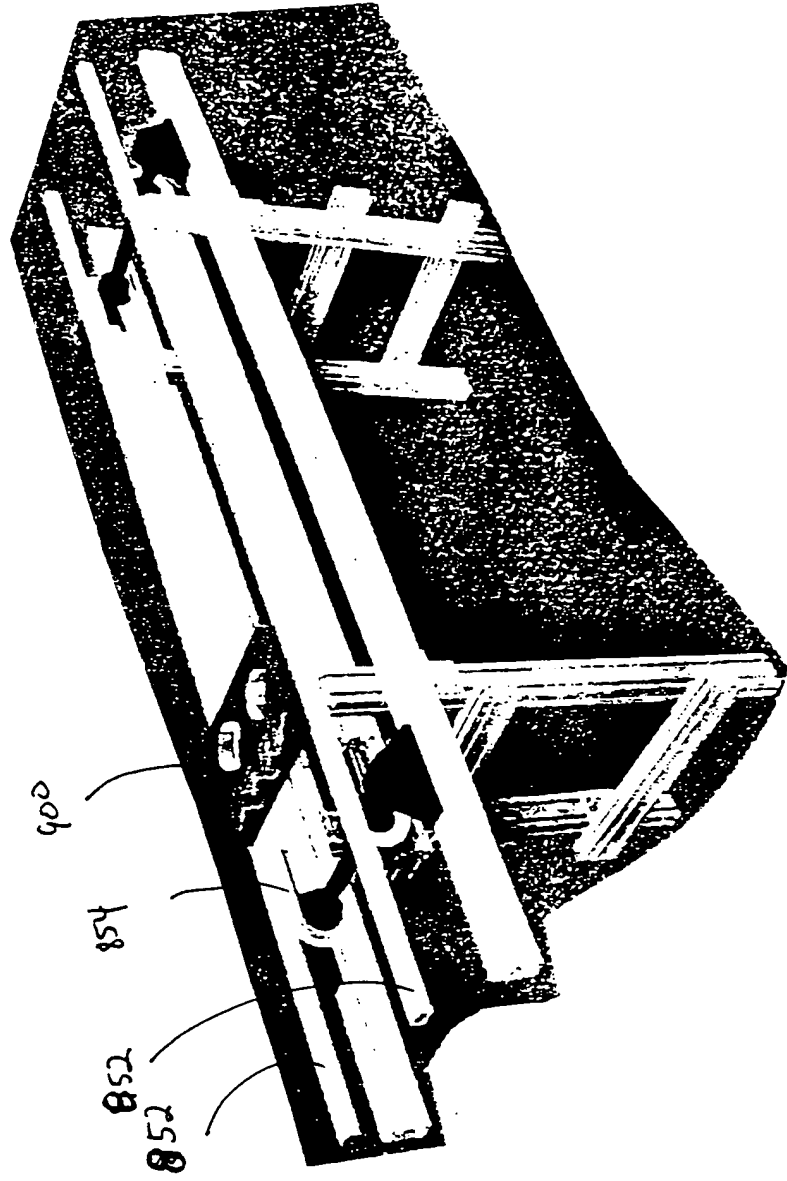


FIG. 31



Fig. 32

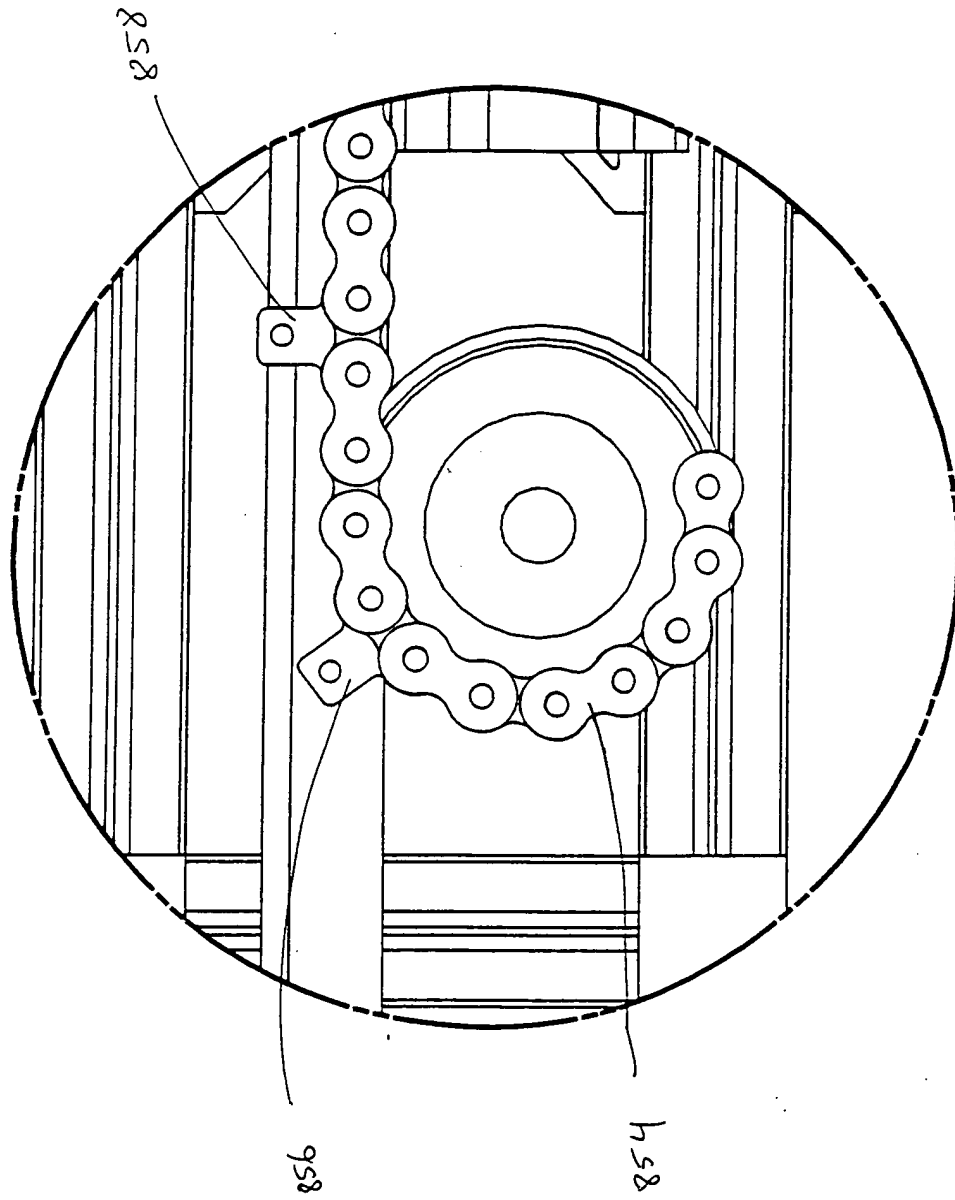


FIG. 33

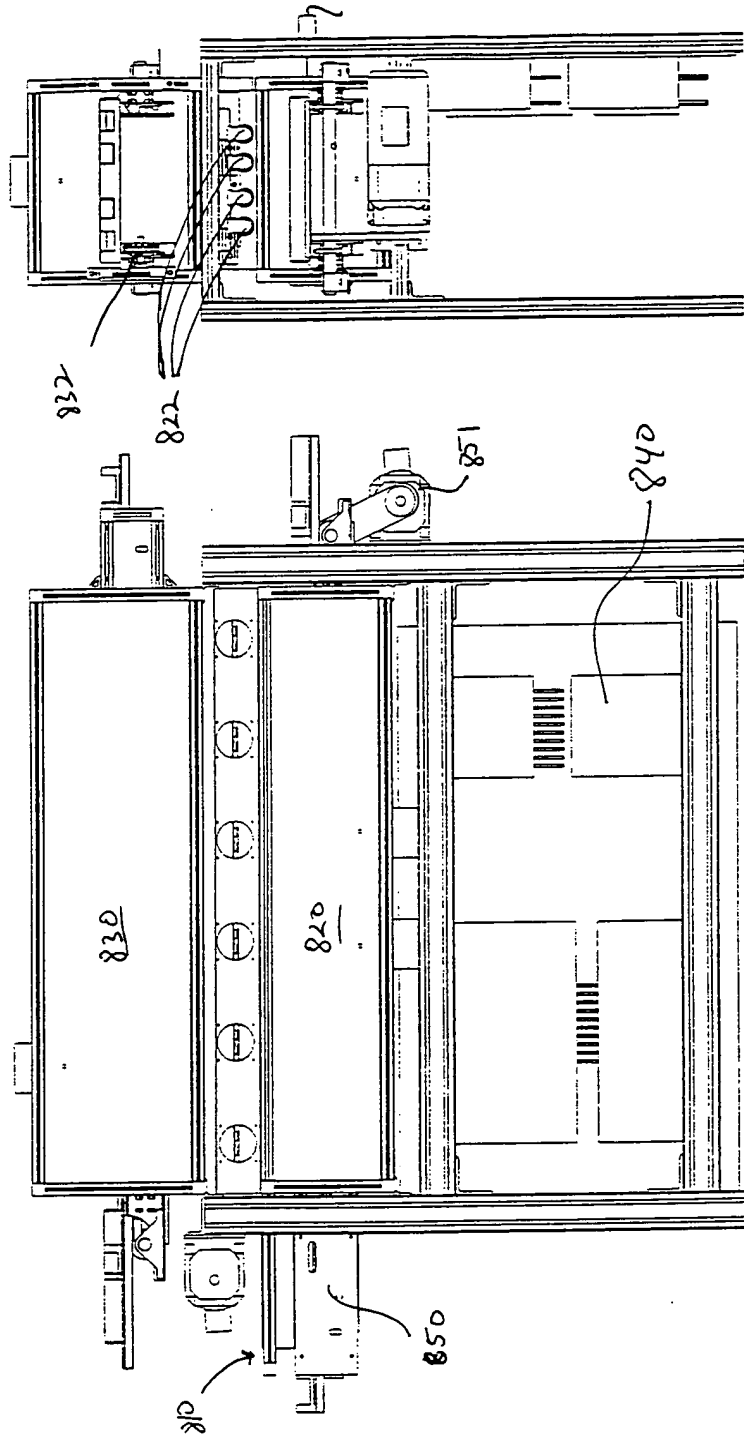


FIG. 35

FIG. 34



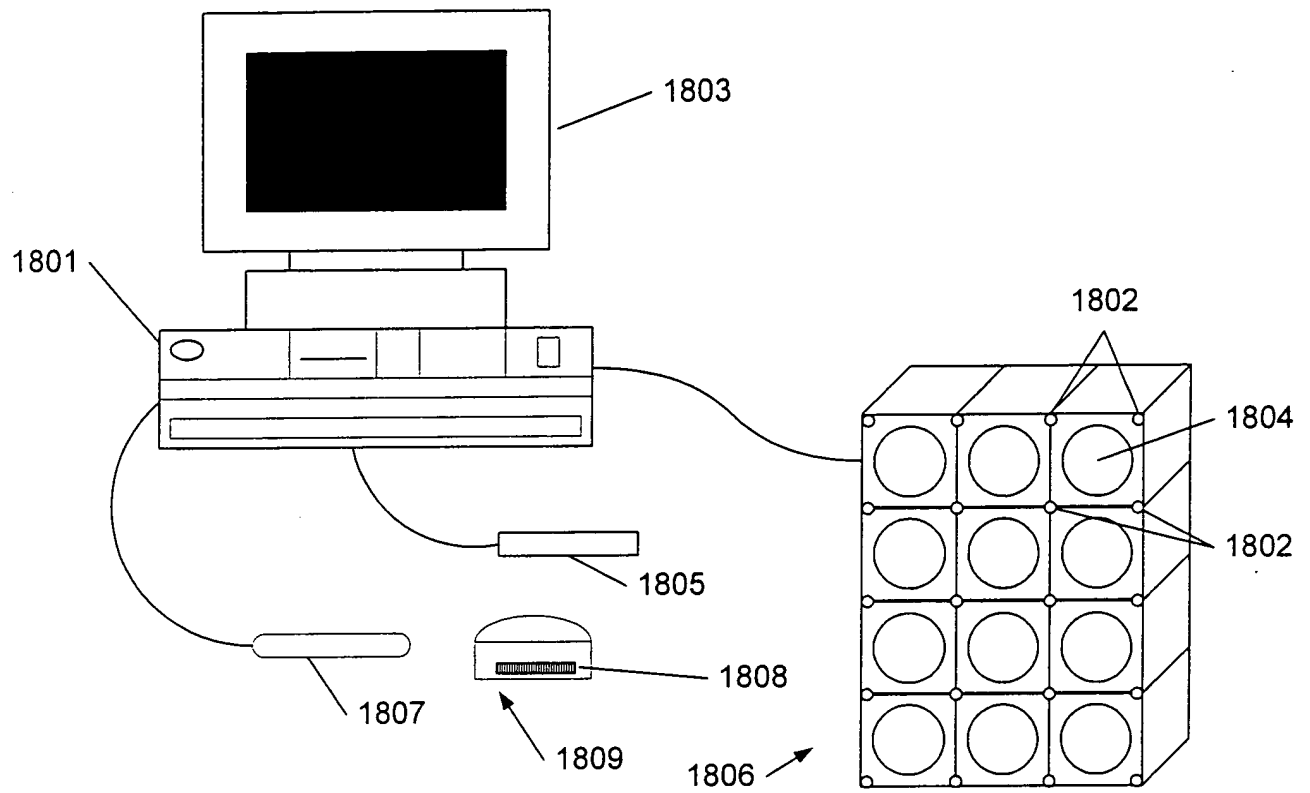


Fig.36

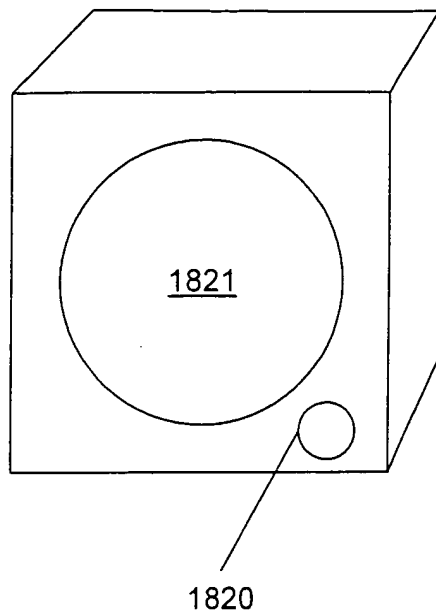

(a)

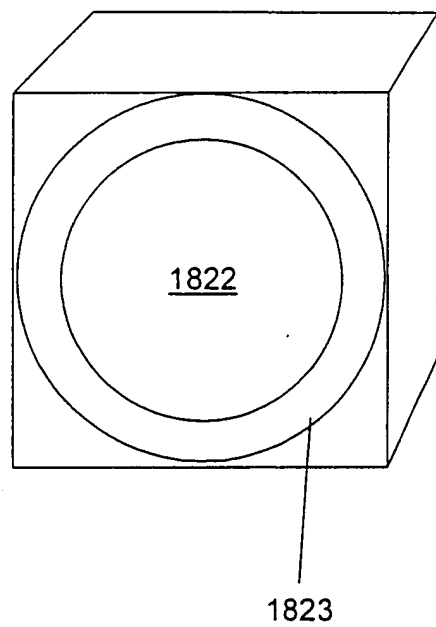

(b)

Fig. 37

TOP SECRET

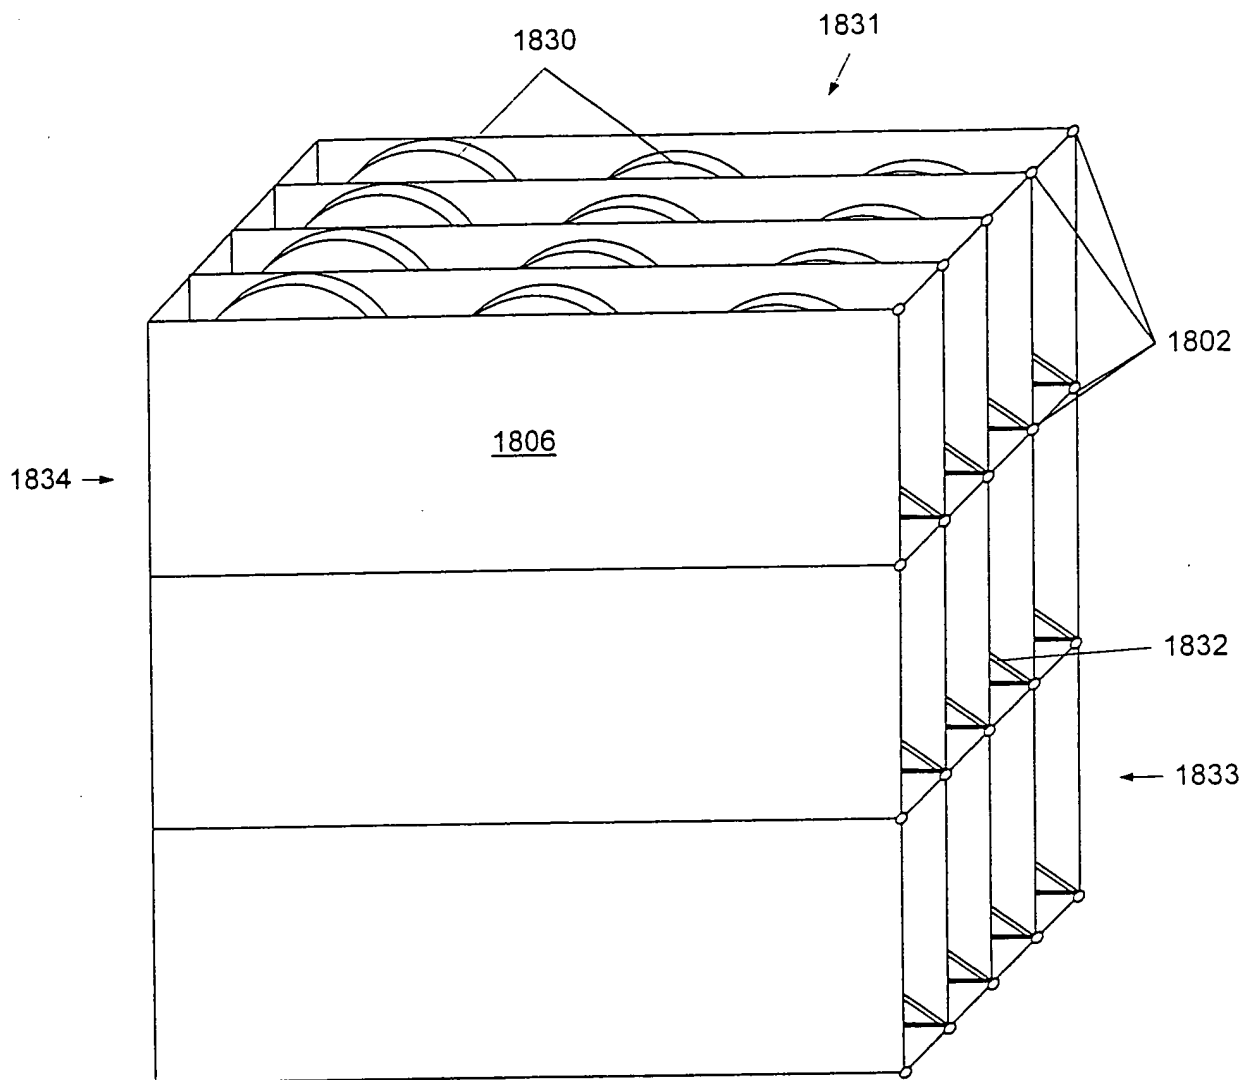


Fig. 38



FIG. 39


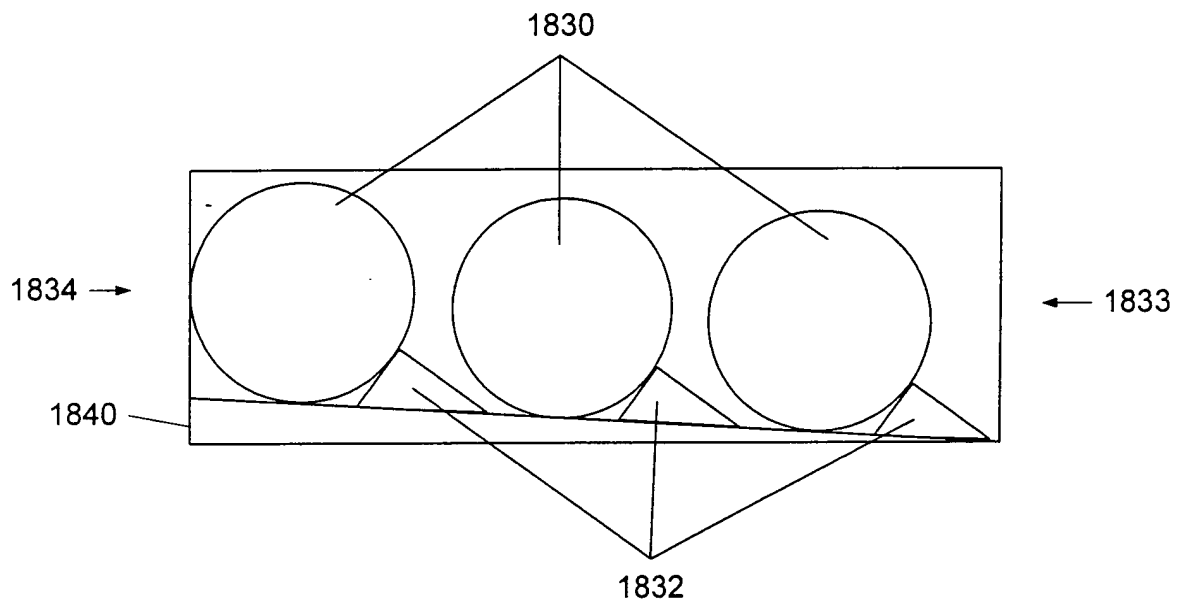


Fig. 39

FIG. 40

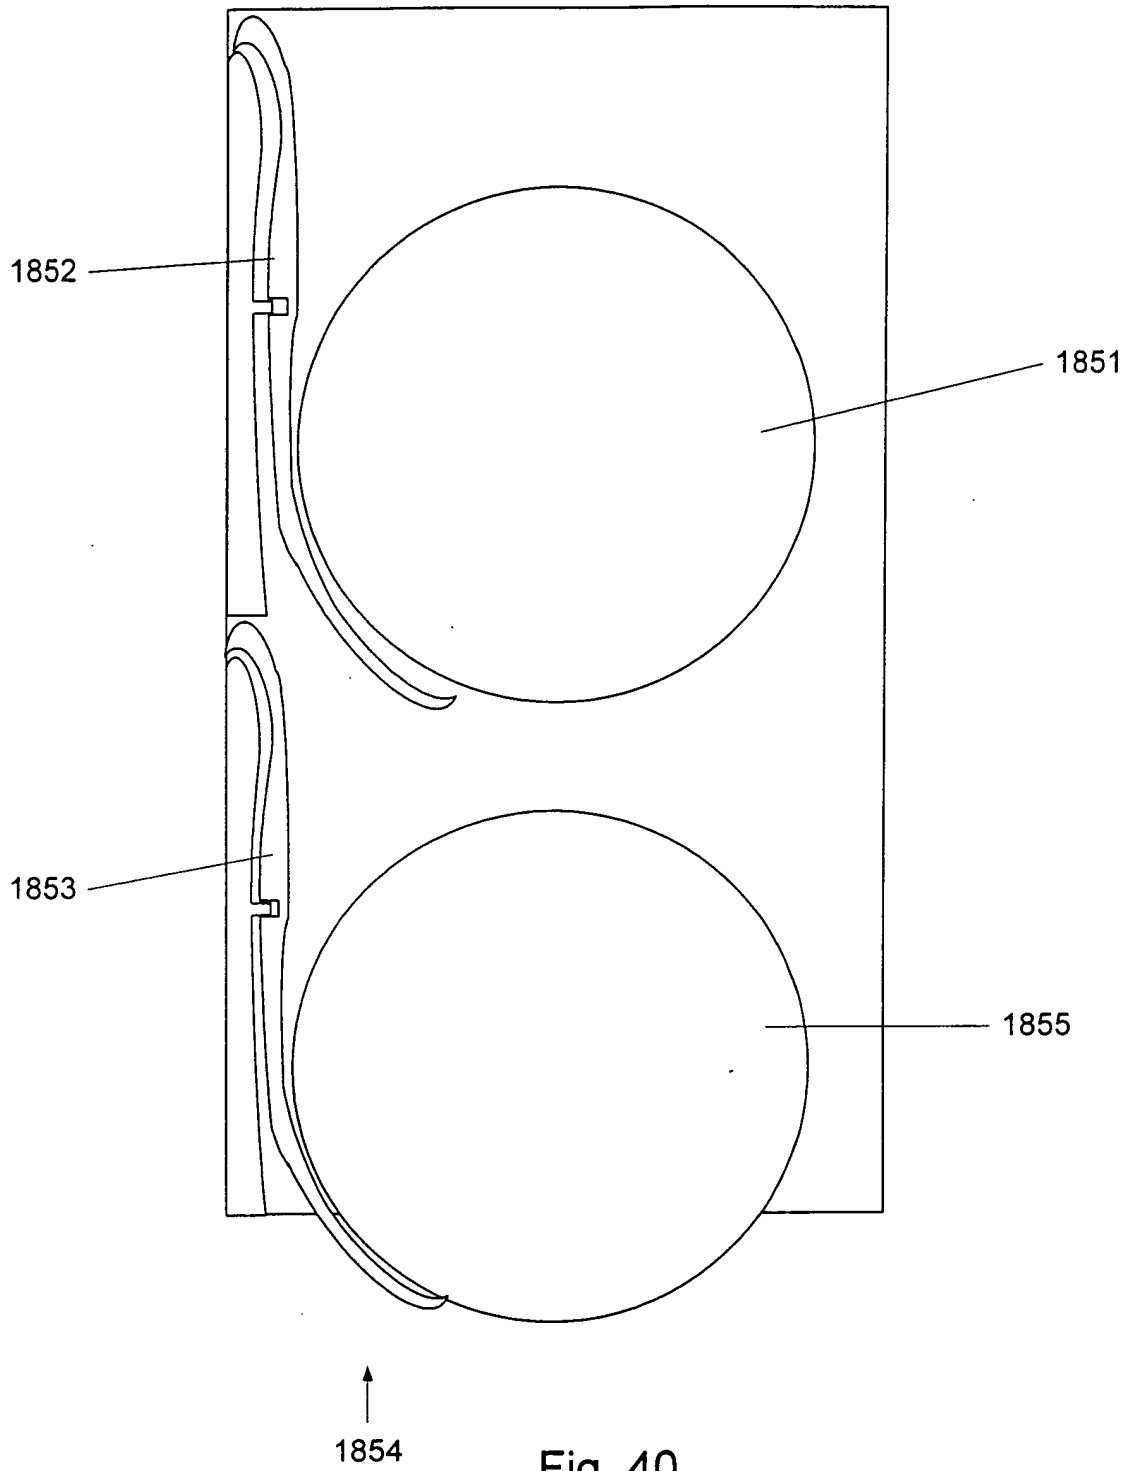

102720 6E488260

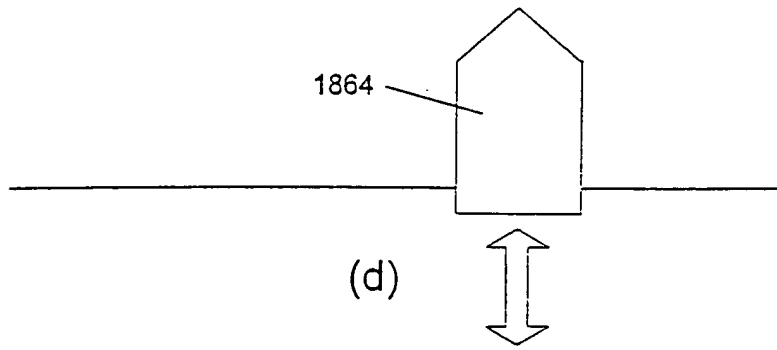
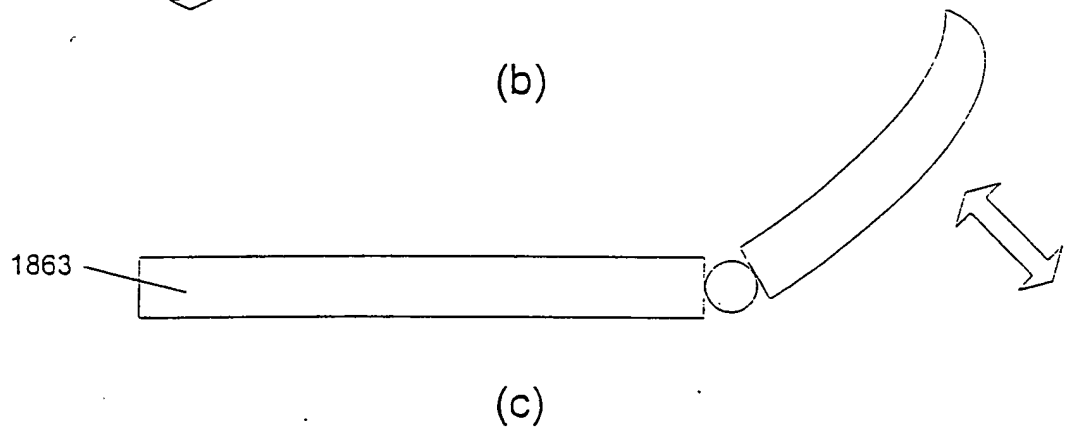
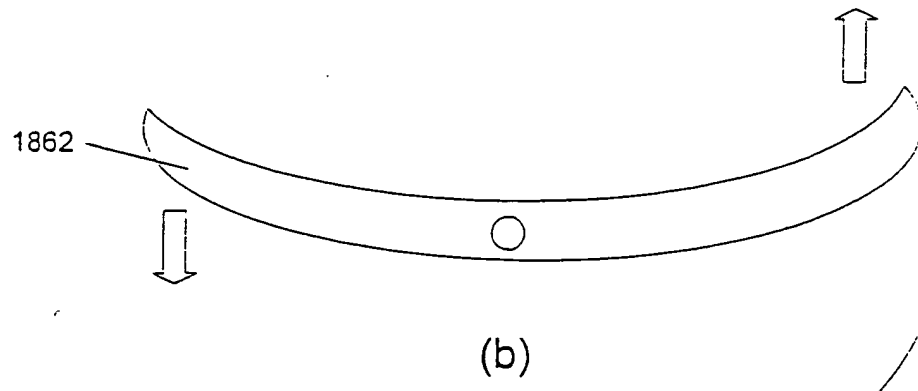
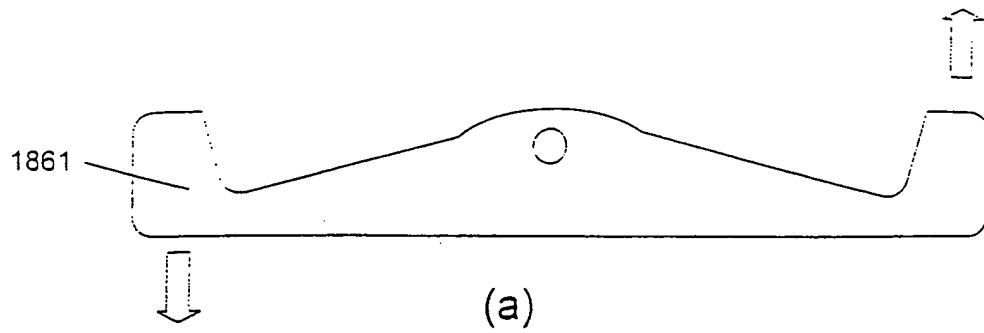


Fig. 41



Fig. 42

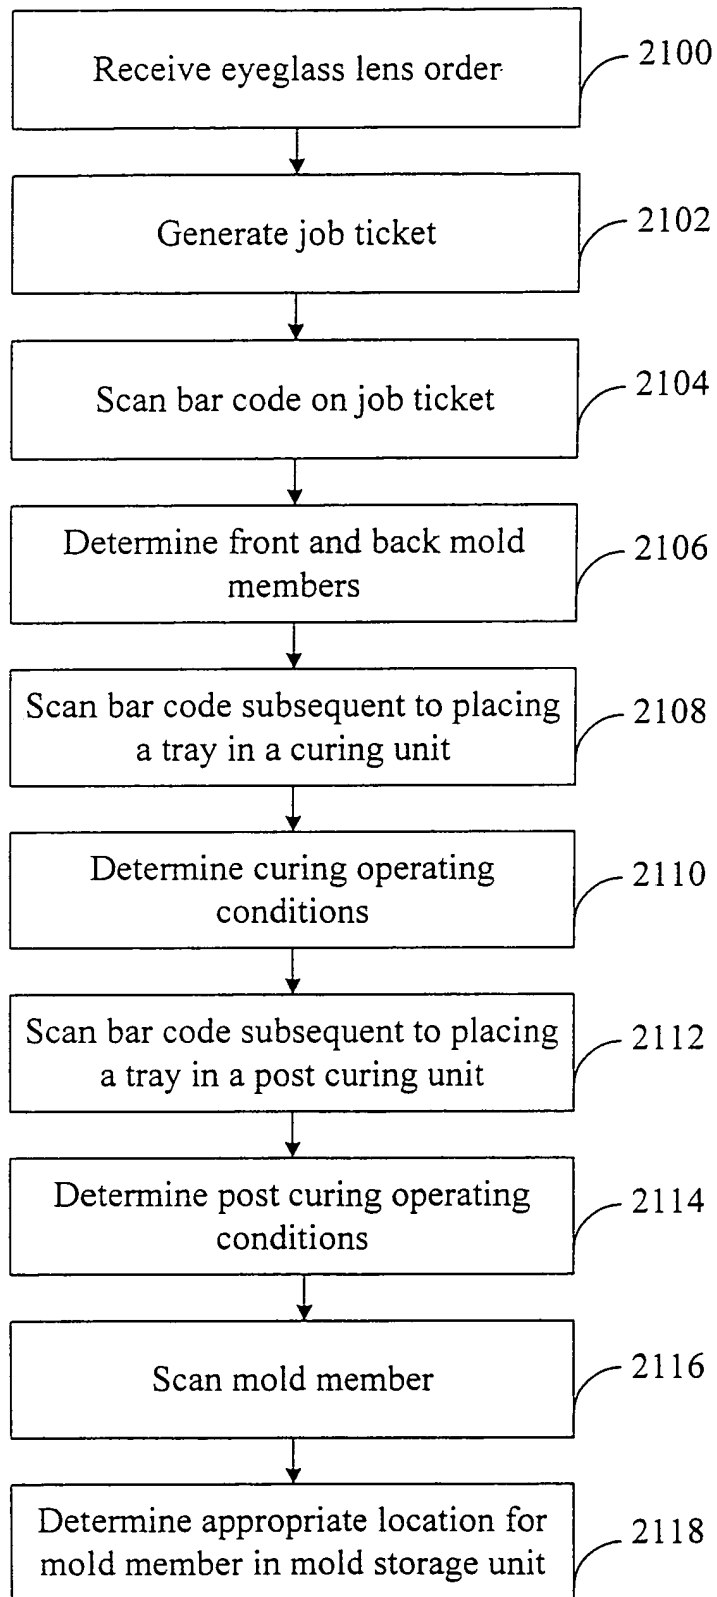


Fig. 43

FOOTNOTES

2202 2204 2206

*optical dynamics*

2208

2210

2214

2216

2218

2200

2228

2226

2212

2222

2224

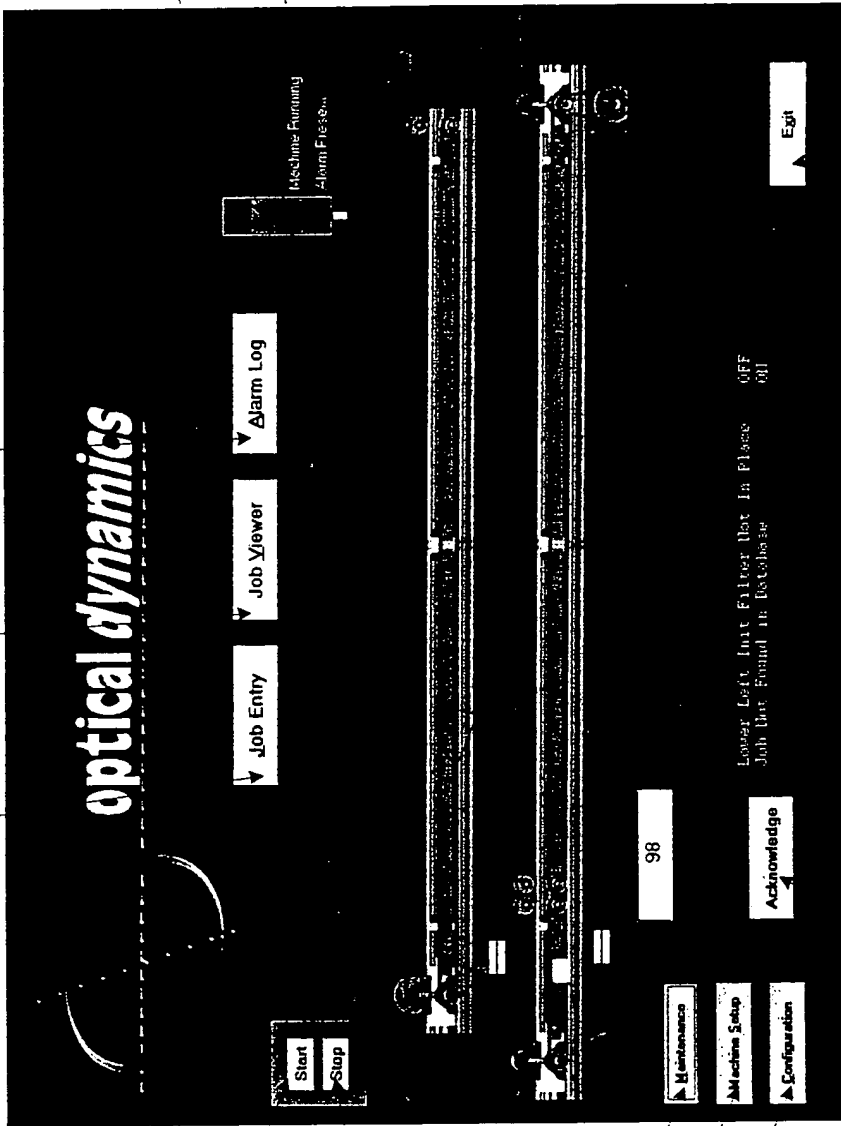


Fig. 44

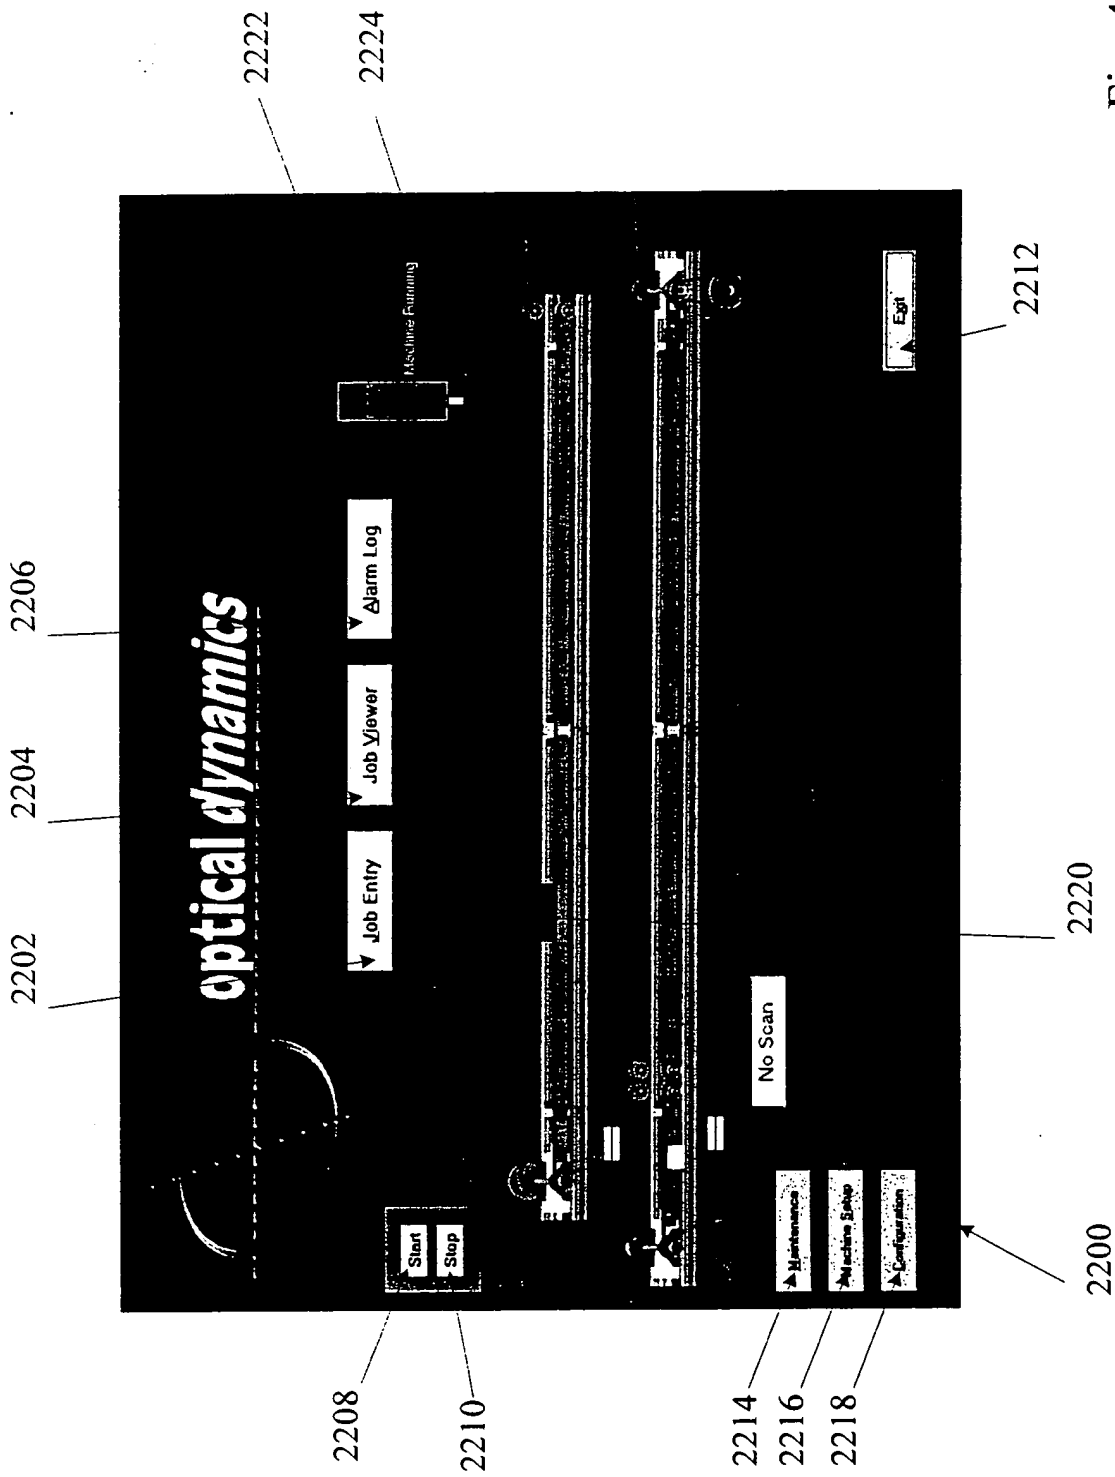


Fig. 45

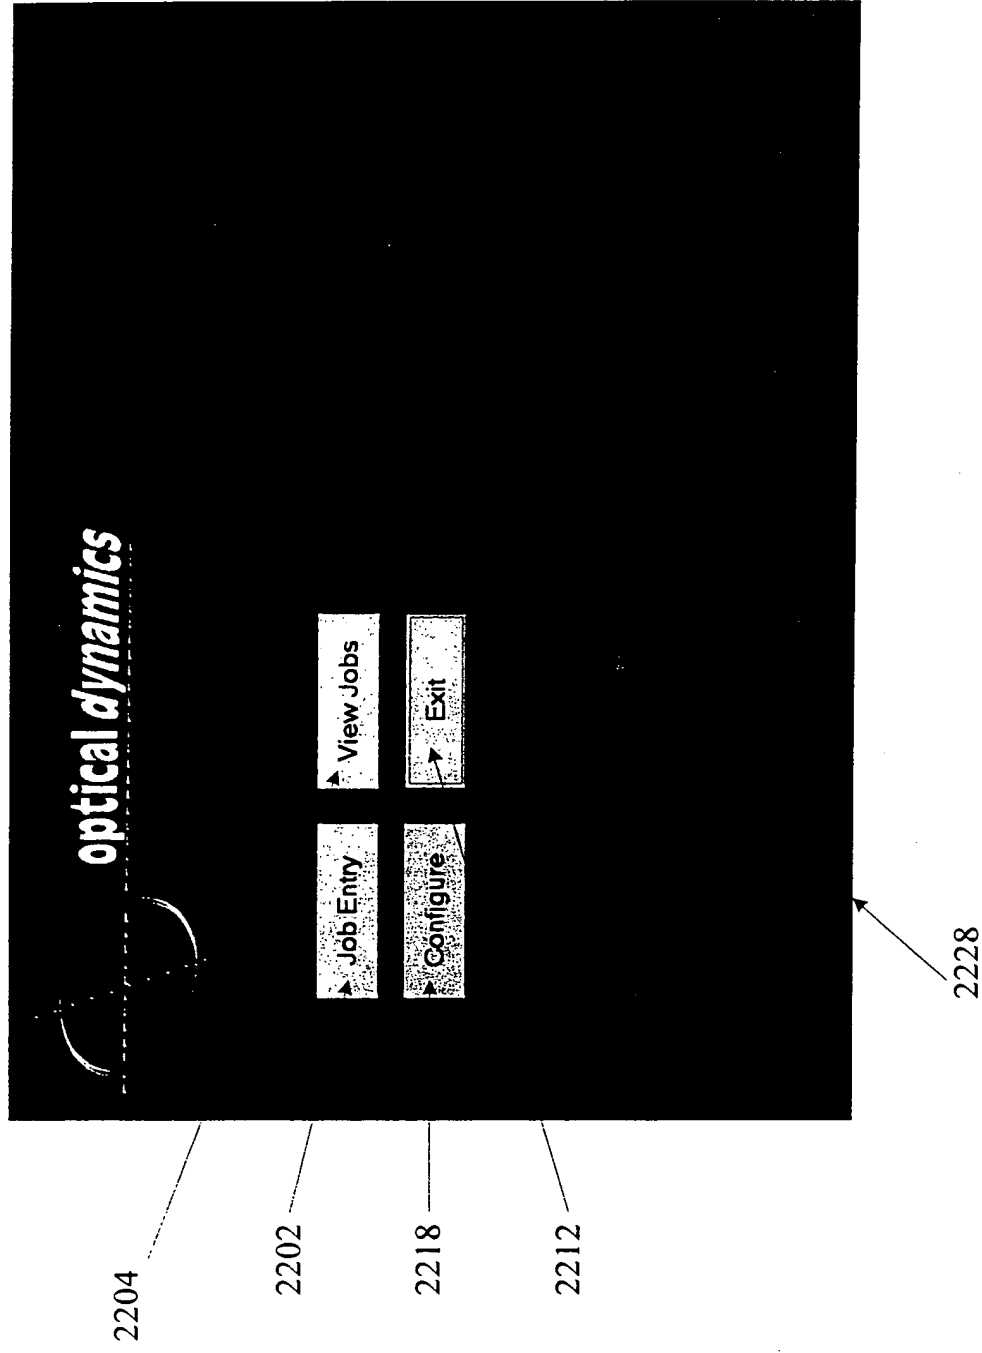


Fig. 46



Job Entry

Job #

Patient Name

Tray #

Bin Location

Priority

Normal

Re-Work

Job Type

Right & Left Lens

Right Lens Only

Left Lens Only

Lens Type

Aspheric - Single Vision

Flat Top

Paradigm Progressive

Monomer/Tint

Clear

Clear w/ Tint

Grey

Right Eye

Sphere

Cylinder

Left Eye

Sphere

Cylinder

Cancel Entry

Create Job

2232

2234

2236

2238

2240

2230

Fig. 47

FOET 20 05:33 PM

Job Viewer

2244

LMS Job #

Patient

2246

LMS Tray #

Entry Date

Bin Location

Lens Type

Monomer

Rx

Left

Right

Power

Cylinder

Axis

Add

Transposed

Molds

Left

Right

Front

Back

Gasket

Filter

Recipe

2248

Re-Print

2280

Close

Fig. 48

FIG. 49

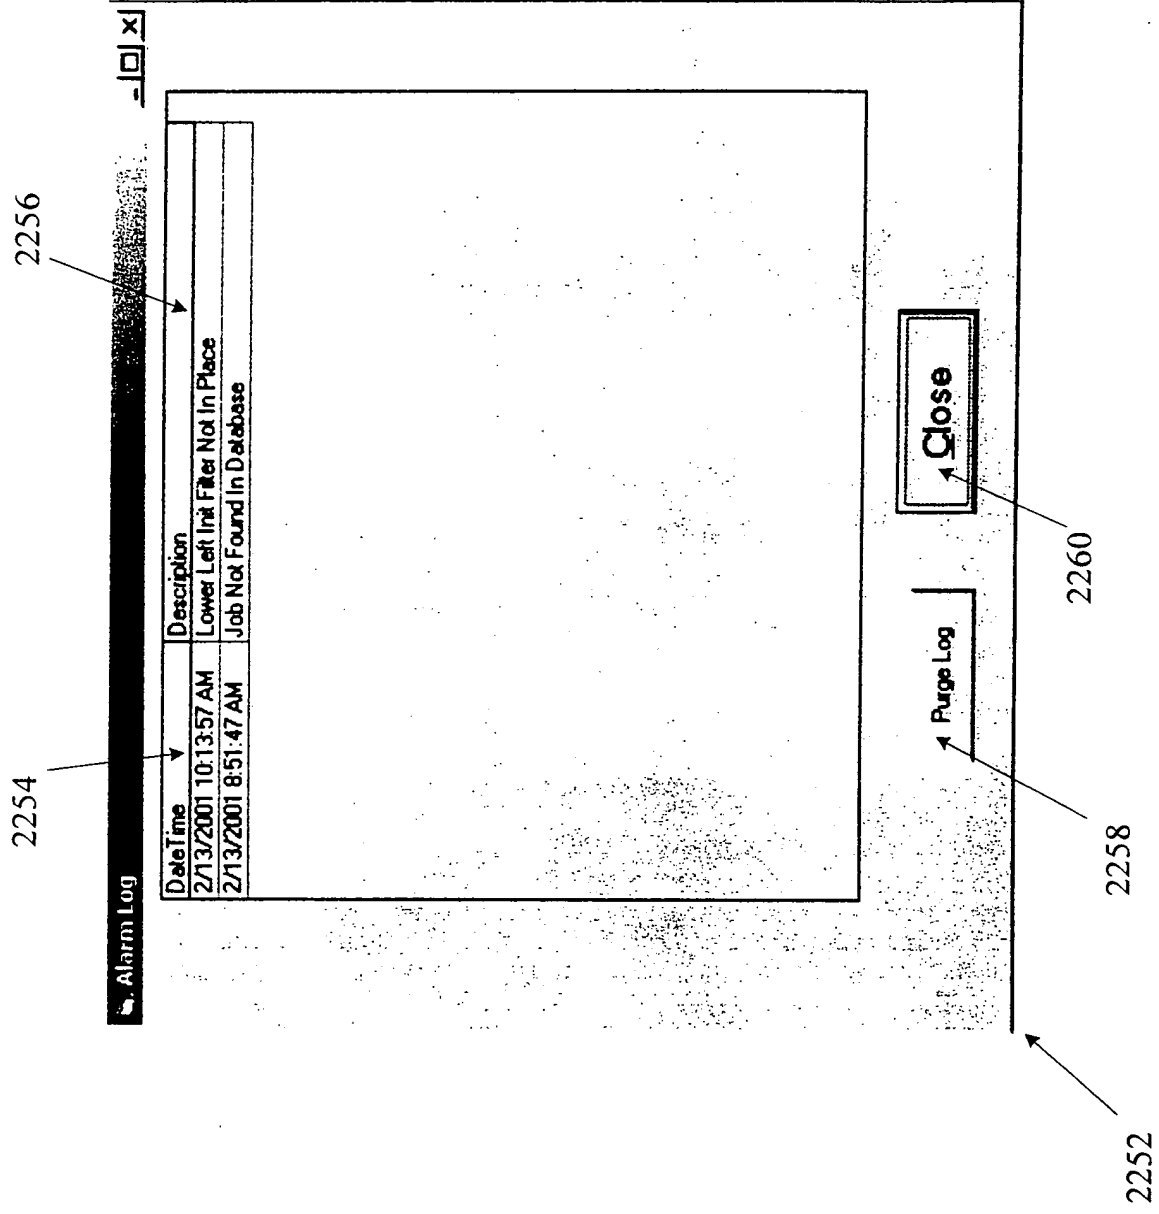


Fig. 49

FIG. 50

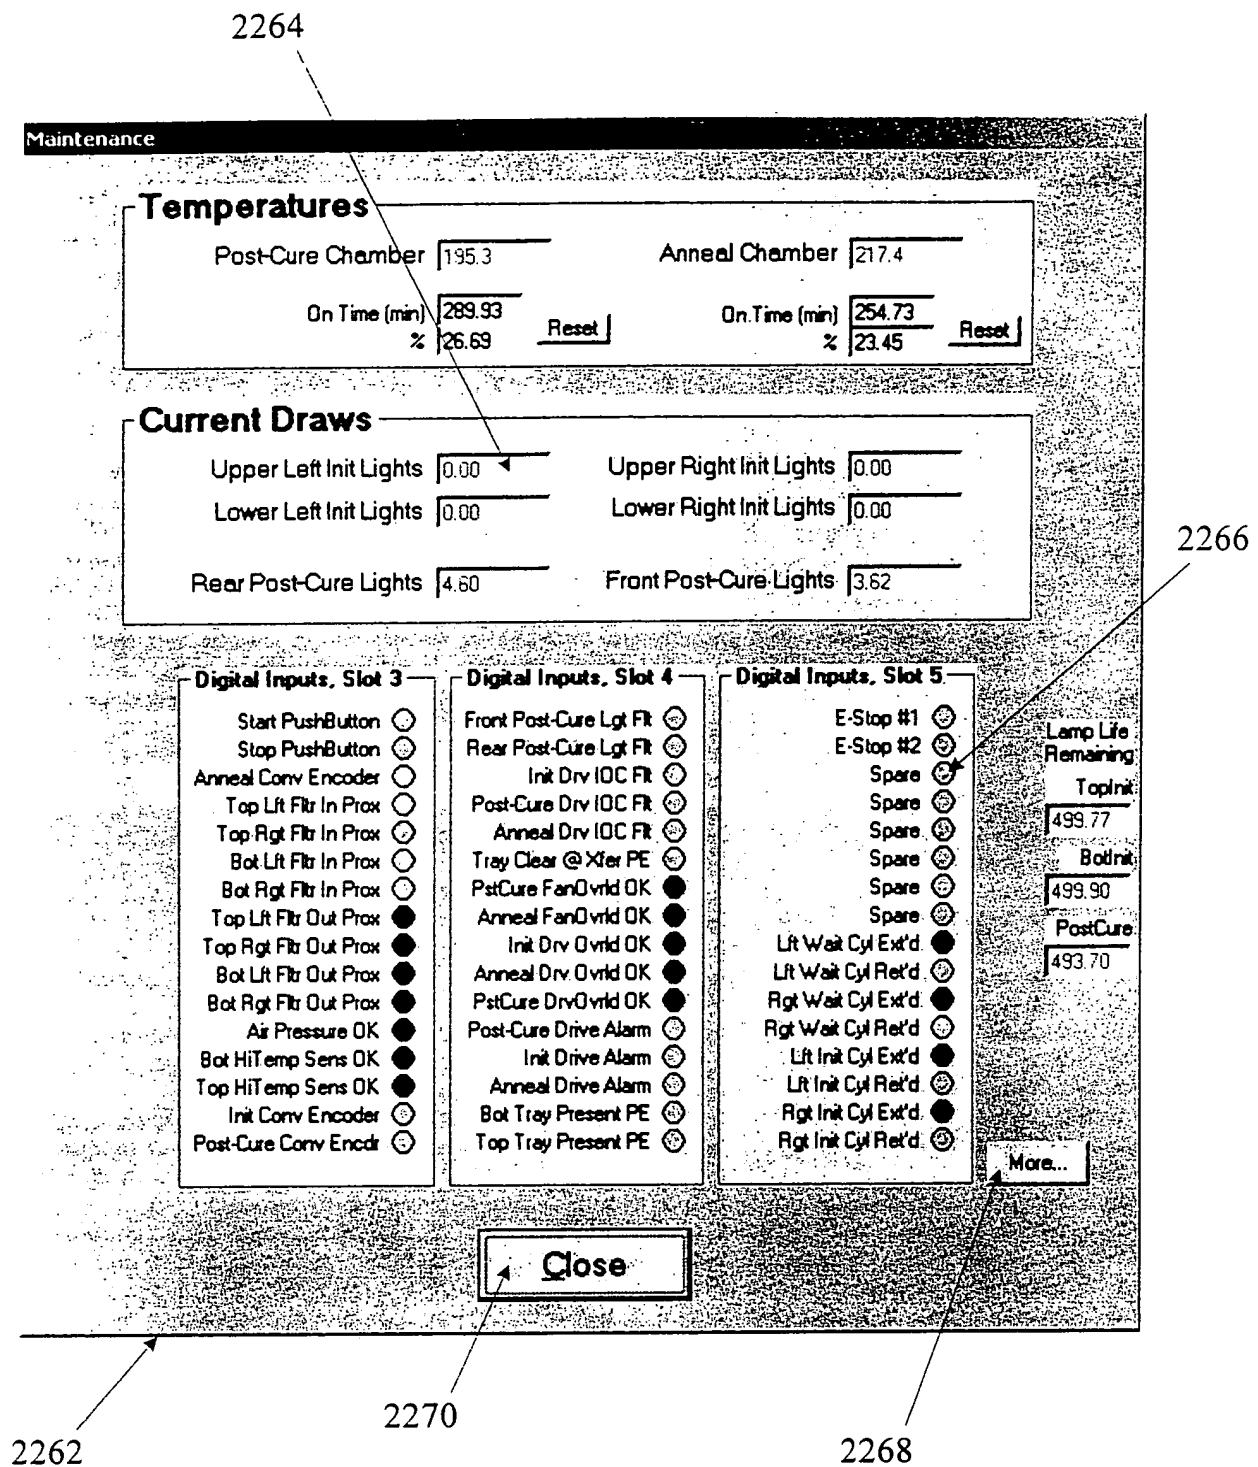


Fig. 50

FIG. 51

2274

**Machine Setup**

**Anneal Conveyor**

High Temp Alarm Limit

Temperature Setpoint

Low Temp Alarm Limit

**Post-Cure Conveyor**

High Temp Alarm Limit

Temperature Setpoint

Low Temp Alarm Limit

**Initialization Lights**

High Current Alarm Limit

Low Current Alarm Limit

No Scan Upper Init Time

No Scan Lower Init Time

No Scan Filter Select ☐

**Post-Cure Lights**

High Current Alarm Limit

Low Current Alarm Limit

**Lamp Maintenance**

Replaced Top Init Lamps ☐

Replaced Bot Init Lamps ☐

Replaced Post-Cure Lamps ☐

**Save Changes** **Cancel Changes**

2272 2278 2280 2276

Fig. 51

2282

Recipe DB: [C:\OptDyn\MGR112700.mdb] Browse... 2284 2286 2288

Job DB: [C:\OptDyn\JobTickets.mdb] Browse... 2290

Ticket Dir: [C:\OptDyn\] Browse... 2292

Ticket Poll Rate (sec) [2] 2294

Ticket Print Scale (%) [100]

Archive Jobs Every [14] Days Keeping [3] Days

v1.05 Cancel OK

Fig. 52

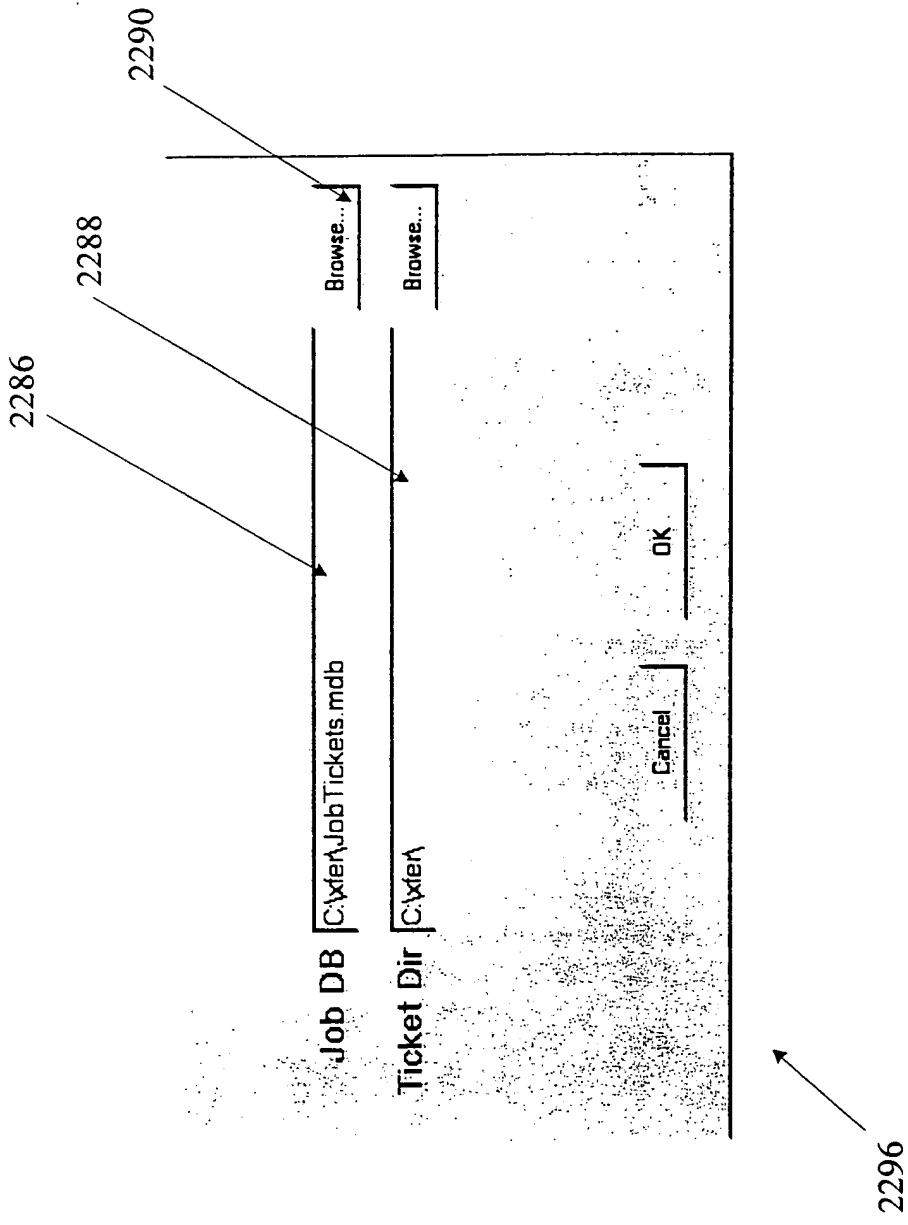


Fig. 53